

# 3.0GHz Spectrum Analyzer

GSP-830

---

## USER MANUAL

GW INSTEK PART NO. 82SP-83000MA1



ISO-9001 CERTIFIED MANUFACTURER

**GW INSTEK**

This manual contains proprietary information, which is protected by copyrights. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will company.

The information in this manual was correct at the time of printing. However, Good Will continues to improve products and reserves the rights to change specification, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd.

No. 7-1, Jhongsing Rd., Tucheng City, Taipei County 236, Taiwan.

# Table of Contents

<b>SAFETY INSTRUCTIONS .....</b>	<b>7</b>
Safety Symbols .....	7
Safety Guidelines .....	8
<b>GETTING STARTED .....</b>	<b>11</b>
GSP-830 Characteristics .....	12
Package Contents .....	13
Front Panel Overview .....	14
Rear Panel Overview .....	17
Display Overview .....	20
Tilt Stand & Power Up .....	22
Error Check .....	23
Functionality Check .....	24
<b>QUICK REFERENCE .....</b>	<b>26</b>
Operation Shortcuts .....	27
Menu Tree .....	33
Preset Contents .....	41
<b>FREQUENCY/SPAN .....</b>	<b>42</b>
View Signal (Center and Span) .....	43
View Signal (Start and Stop) .....	45
Full/Zero Span .....	47
Recall the Last Span Setting .....	48
<b>AMPLITUDE .....</b>	<b>49</b>
Set Vertical Scale .....	50
Amplitude Correction .....	53
Use Pre-Amplifier GAP-801 (Optional) .....	58
Set Input Impedance .....	59
<b>AUTOSET .....</b>	<b>60</b>
<b>MARKER .....</b>	<b>63</b>

Activate/de-activate marker(s).....	64
Move marker(s).....	67
Show Markers in Table.....	69
<b>PEAK SEARCH .....</b>	<b>70</b>
Search Signal Peaks.....	71
Show Peak Table.....	73
<b>TRACE .....</b>	<b>75</b>
View traced waveform.....	76
Move Marker to Trace.....	78
Run Trace Math.....	80
Select Signal Detection Mode.....	82
<b>POWER MEASUREMENT.....</b>	<b>84</b>
ACPR Measurement.....	85
OCBW Measurement.....	88
N dB Measurement.....	90
Phase Jitter Measurement.....	91
<b>LIMIT LINE .....</b>	<b>92</b>
Edit Limit Line.....	93
Run Pass/Fail test.....	96
<b>BANDWIDTH .....</b>	<b>98</b>
Select RBW (Resolution BandWidth).....	99
Select VBW (Video BandWidth).....	101
RBW/VBW Auto Mode Contents.....	102
Set Sweep time.....	104
Average Waveform.....	104
<b>TRIGGER.....</b>	<b>106</b>
<b>DISPLAY.....</b>	<b>110</b>
Change Display Brightness.....	111
Activate Display Line.....	111
Enter Display Title.....	112
Use Split Display.....	113

Use VGA Output .....	114
Save Display Image to USB Flash Drive.....	114
<b>FILE .....</b>	<b>116</b>
File Location and File Type .....	117
File Copy Step.....	118
File Delete Step.....	121
File Rename Step .....	123
Save Display Image to USB Flash Drive.....	124
<b>PRESET .....</b>	<b>126</b>
<b>SYSTEM.....</b>	<b>127</b>
Save/Recall Panel Setting .....	128
Configure Communication Interface.....	129
View System Information.....	131
Set Date/Time.....	135
Synchronize GSP-830 with Other Device.....	136
Select Menu Language.....	138
Service operation menu .....	138
<b>SEQUENCE.....</b>	<b>139</b>
Edit Sequence.....	140
Run Sequence.....	143
<b>TRACKING GENERATOR.....</b>	<b>145</b>
<b>DEMODULATOR .....</b>	<b>147</b>
<b>EMI FILTER .....</b>	<b>149</b>
<b>BATTERY / DC OPERATION .....</b>	<b>151</b>
Battery Operation.....	151
DC Operation .....	152
<b>PC SOFTWARE.....</b>	<b>153</b>
Install Software .....	154

Connect Software .....	155
Use Software .....	158
<b>REMOTE CONTROL.....</b>	<b>161</b>
Configure Interface .....	162
Command Syntax.....	164
Command Set.....	165
<b>FAQ.....</b>	<b>178</b>
<b>Appendix.....</b>	<b>180</b>
GSP-830 Specification.....	180
Optional Items Specifications .....	182
Declaration of Conformity.....	184
<b>INDEX .....</b>	<b>185</b>







## SAFETY INSTRUCTIONS

This chapter contains important safety instructions that you must follow when operating GSP-830 and when keeping it in storage. Read the following before any operation to insure your safety and to keep the best condition for GSP-830.



## Safety Symbols

These safety symbols may appear in this manual or on GSP-830.

	<b>WARNING</b>	Warning: Identifies conditions or practices that could result in injury or loss of life.
	<b>CAUTION</b>	Caution: Identifies conditions or practices that could result in damage to GSP-830 or to other properties.
	<b>DANGER</b>	High Voltage
	<b>ATTENTION</b>	Refer to the Manual
	<b>PC</b>	Protective Conductor Terminal
	<b>ET</b>	Earth (ground) Terminal

## Safety Guidelines

---

### General Guideline



#### CAUTION

- Make sure that the RF input level and the Tracking Generator output reversed power level do not exceed +30dBm.
- Do not supply an input signal to the Tracking Generator output.
- Do not place any heavy object on GSP-830.
- Avoid severe impacts or rough handling that leads to damaging GSP-830.
- Do not discharge static electricity to GSP-830.
- Use only mating connectors, not bare wires, for the terminals.
- Do not block or obstruct the cooling fan vent opening.
- Do not perform measurement at power source and building installation site (Note below).
- Do not disassemble GSP-830 unless you are qualified as service personnel.

---

(Note) EN 61010-1:2001 specifies the measurement categories and their requirements as follows. GSP-830 falls under category II.

- Measurement category IV is for measurement performed at the source of low-voltage installation.
- Measurement category III is for measurement performed in the building installation.
- Measurement category II is for measurement performed on the circuits directly connected to the low voltage installation.

### Power Supply



#### WARNING

- AC Input voltage: 100 ~ 240 V AC, 50/60Hz
- DC Input voltage: 12V DC, 40W maximum
- The power supply voltage should not fluctuate more than 10%.
- Connect the protective grounding conductor of the AC power cord to an earth ground, to avoid electrical shock.


### Battery



#### CAUTION

- Rating: 10.8V Li-Ion battery pack x 2
- Turn Off the main power switch before installing or taking out the battery packs.



Fuse  WARNING	<ul style="list-style-type: none"> <li>• Fuse type: T1.6A/ 250V</li> <li>• Make sure the correct type of fuse is installed before power up.</li> <li>• To ensure fire protection, replace the fuse only with the specified type and rating.</li> <li>• Disconnect the power cord before fuse replacement.</li> <li>• Make sure the cause of fuse blowout is fixed before fuse replacement.</li> </ul>
Cleaning GSP-830	<ul style="list-style-type: none"> <li>• Disconnect the power cord before cleaning.</li> <li>• Use a soft cloth dampened in a solution of mild detergent and water. Do not spray any liquid into GSP-830.</li> <li>• Do not use chemical or cleaner containing harsh material such as benzene, toluene, xylene, and acetone.</li> </ul>
Operation Environment	<ul style="list-style-type: none"> <li>• Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (Note below)</li> <li>• Relative Humidity: &lt; 90%</li> <li>• Altitude: &lt; 2000m</li> <li>• Temperature: 18°C to 28°C</li> </ul> <p>(Note) EN 61010-1:2001 specifies the pollution degrees and their requirements as follows. GSP-830 falls under degree 2. Pollution refers to “addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity”.</p> <ul style="list-style-type: none"> <li>• Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence.</li> <li>• Pollution degree 2: Normally only non-conductive pollution occurs. Occasionally, however, a temporary conductivity caused by condensation must be expected.</li> <li>• Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled.</li> </ul>
Storage Environment	<ul style="list-style-type: none"> <li>• Location: Indoor</li> <li>• Relative Humidity: &lt; 85%</li> <li>• Temperature: 0°C to 40°C</li> </ul>

## Power cord for the United Kingdom

When using GSP-830 in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead / appliance must only be wired by competent persons



**WARNING: THIS APPLIANCE MUST BE EARTHED**

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

Green/ Yellow: Earth

Blue: Neutral

Brown: Live (Phase)



As the colours of the wires in main leads may not correspond with the colours marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with the letter E or by the earth symbol  $\oplus$  or coloured Green or Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, cable of 0.75mm<sup>2</sup> should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any moulded mains connector that requires removal /replacement must be destroyed by removal of any fuse & fuse carrier and disposed of immediately, as a plug with bared wires is hazardous if engaged in live socket. Any re-wiring must be carried out in accordance with the information detailed on this label.

# GETTING STARTED

This chapter describes GSP-830 in a nutshell, including its main features, package contents, and front / rear / display panel introduction. After going through the overview, follow the Power-up sequence and Functionality check section to properly setup GSP-830.



GSP-830 package	GSP-830 Characteristics .....	12
	Package Contents.....	13
Panel introduction	Front Panel Overview .....	14
	Rear Panel Overview .....	17
	Display Overview .....	20
	Status Icon Overview .....	21
Setup	Tilt stand .....	22
	Power Up.....	22
	Error Check .....	23
	Functionality Check.....	24

## GSP-830 Characteristics

GSP-830 is a middle- to high-range digital storage spectrum analyzer suitable for wide range of applications, such as production testing, research, and field verification.

Performance	<ul style="list-style-type: none"> <li>• Low noise floor: -117dBm @600MHz, 3k RBW</li> <li>• Fast sweep: 50ms ~ 25.6s range</li> <li>• Compact size: 330(W) x 170(H) x 340(D) mm</li> <li>• Light weight: 5.8kg (without options)</li> </ul>
Features	<ul style="list-style-type: none"> <li>• Autoset</li> <li>• 5 markers with Delta Marker and Peak functions</li> <li>• 3 traces</li> <li>• Power measurements: ACPR, OCBW, N-dB, Phase Jitter</li> <li>• Pass/Fail test with Limit Line editing</li> <li>• Split windows with separate settings</li> <li>• Sequence programming (user-defined macro)</li> <li>• 6.4" TFT color LCD, 640 x 480 resolution</li> <li>• Phone output (available in optional Demodulator)</li> <li>• AC/DC/Battery multi-mode power operation</li> </ul>
Interface	<ul style="list-style-type: none"> <li>• USB host for storage device connection</li> <li>• USB slave/RS232/GPIB(optional) for PC software connection and remote control</li> <li>• Direct VGA display image output</li> <li>• Reference signal input/output for synchronization</li> <li>• External trigger signal input</li> </ul>
Optional Items	<ul style="list-style-type: none"> <li>• Tracking Generator</li> <li>• Pre-Amplifier (11.5dB, 6GHz)</li> <li>• <math>\pm 1</math>ppm stability module</li> <li>• EMI filter with 9kHz/120kHz RBW and 6-dB bandwidth</li> <li>• Battery pack</li> <li>• Demodulator</li> <li>• 300Hz/10kHz/100kHz RBW</li> <li>• GPIB interface</li> </ul>

## Package Contents

Contact your dealer in case there is a missing item.

GSP-830 + pre-installed  
optional items



The following, if bundled, are factory installed items.

- Option01 Tracking Generator
- Option03  $\pm 1$ ppm Stability module
- Option04 300Hz RBW
- Option05 9kHz & 120kHz RBW (\*)
- Option06 10/100kHz RBW (\*)
- Option07 AM/FM Demodulator, 10/100kHz RBW (\*)

\* Among Option 05 ~ 07, only one can be installed at a time.

Peripherals

- Power cord
- User Manual (this document)

Other Optional items

Option02 Battery Packs\*2

Option08 GPIB Interface

GSC-001 Soft carrying case

GKT-001 General Kit set

ADP-002: SMA (J/F) to N (P/M) adaptor x 2

ATN-100: 10dB Attenuator

GTL-303: RF Cable assembly (RD316+SMA(P)x2,60cm)x2

GSC-002: Kit box

GKT-002 CATV Kit set

ADP-001: BNC (J/F) to N (P/M) adaptor x 2

ADP-101: BNC(P/M) 50 $\Omega$  to BNC(J/F) 75 $\Omega$  adaptor x2

GTL-304: RF Cable assembly (RG223,N(P)-N(J),30cm)x2

GSC-003: Kit box

GKT-003 RLB Kit set

GAK-001: Cal. Kit, termination, N(P), 50 $\Omega$

GAK-002: Cap with chain, N(P)

GTL-302: RF Cable assembly (RG223+N(P)x2, 30cm) x2

GSC-004: Kit box


GAP-801 Pre-Amplifier, 9kHz ~ 6GHz, 10dB gain

GKT-006 EMI Probe Set











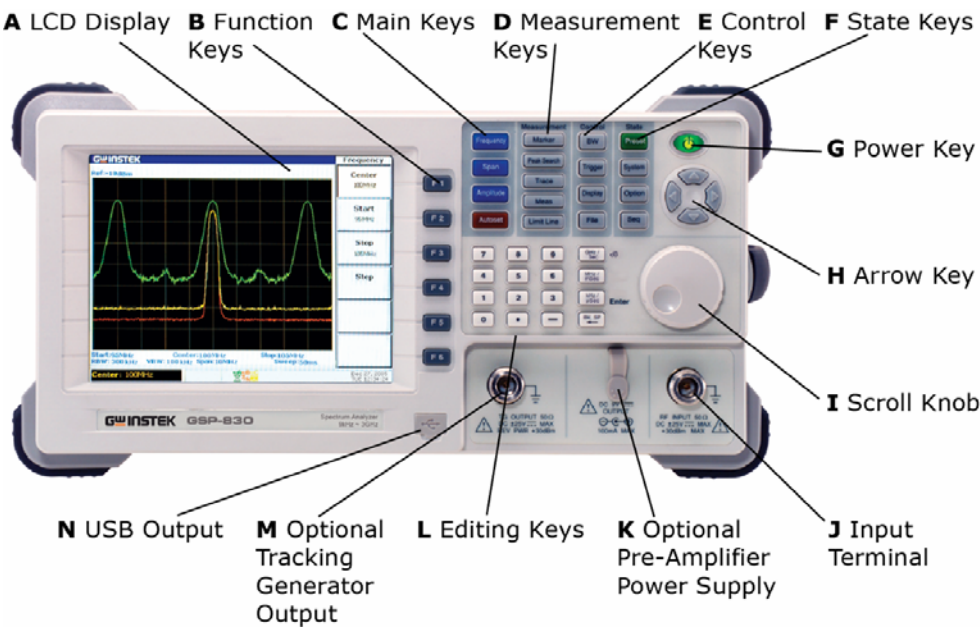


GTP-3000 RF Probe for EMI Use































































GTL-401 DC Power Cord

Front Panel Overview




A	LCD Display	TFT Color display, 640x480 resolution. For display setting details, see page110.	
B	F1~F6 Function Keys	<div><div>F 1</div><div>F 6</div></div> ~	Soft keys linked to the menu that appears on the right side of the display.
C	Main Keys	<div><div>Frequency</div><div>Span</div><div>Amplitude</div><div>Autoset</div></div>	<p><b>Frequency key</b> (page42), together with <b>Span key</b>, configures horizontal (frequency) scale.</p> <p><b>Amplitude key</b> (page49) configures vertical (amplitude) scale and input impedance.</p> <p><b>Autoset key</b> (page60) automatically configures the most appropriate horizontal and vertical scale for input signal.</p>





D Measurement keys	    	<p><b>Marker key</b> (page63) activates markers and places them on specified locations.</p> <p><b>Peak Search key</b> (page70) searches peak signals and configures peak ranges/orders.</p> <p><b>Trace key</b> (page75) activates trace signals, configures them, and runs trace math operations.</p> <p><b>Measurement key</b> (page84) configures and runs 4 types of power measurements: ACPR, OCBW, N-dB, and Phase jitter.</p> <p><b>Limit Line key</b> (page92) configures high/low limit lines and runs Pass/Fail test.</p>
E Control keys	   	<p><b>BW key</b> (page98) configures RBW/VBW width, sweep time length, and waveform averaging number.</p> <p><b>Trigger key</b> (page106) selects trigger type, sets trigger running mode / delay / frequency, and activates external trigger input.</p> <p><b>Display key</b> (page110) configures LCD dimmer, edits and shows display line/title, and activates split windows.</p> <p><b>File key</b> (page116) saves/recalls/deletes trace waveform, limit line, amplitude correction, sequence (macro), and panel setup. It also saves display image through USB port.</p>
F State Keys	   	<p><b>Preset key</b> (page41or126) resets GSP-830 to a predefined state.</p> <p><b>System key</b> configures date/time (page135), GPIB/RS232C interface (page129), and language (page138). Shows system information (page131) and self test result (page134). Saves/recalls panel setup (page128).</p> <p><b>Option key</b> configures Tracking Generator (page145), Demodulator (page147), Battery (page151), and External reference frequency (page136).</p> <p><b>Seq key</b> (page139) edits and runs sequence (user-defined macro).</p>








G	Power Key		Power key selects the power state between Standby mode (Red LED On) and Power On mode (Green LED On). For main power On/Off, use the Power switch on the rear panel. For power up sequence, see page22.												
H	Arrow Key		Arrow key selects parameters in various occasions; Up/Right for increasing, Down/Left for decreasing.												
I	Scroll Knob		Scroll knob sets or selects parameters in various occasions. In some cases, it works in tandem with the Arrow key.												
J	Input Terminal	 	Input terminal accepts RF input signal. Maximum +30dBm, 50Ω.												
K	Pre-Amplifier Power Supply Terminal	 	Pre-Amplifier power supply terminal provides power for the optional GAP-801 pre-amplifier. For details, see page58.												
L	Numerical Keys	<p>Numerical keys set various parameters. In some cases, they work in tandem with the Arrow key / Scroll knob.</p> <table><tr><th>Example</th><th>Key sequence</th></tr><tr><td>9kHz</td><td>  </td></tr><tr><td>-3.8dB</td><td>     </td></tr><tr><td>1.0mS</td><td>   </td></tr><tr><td>9 + Enter</td><td>  </td></tr><tr><td>Correction</td><td></td></tr></table>		Example	Key sequence	9kHz	  	-3.8dB	     	1.0mS	   	9 + Enter	  	Correction	
Example	Key sequence														
9kHz	  														
-3.8dB	     														
1.0mS	   														
9 + Enter	  														
Correction															
M	TG Output Terminal (Optional)	 	Outputs the optional Tracking Generator signal. Reversed power should not exceed +30dBm. For details, see page145.												
N	USB Output Connector	 	USB host, typeA, male connector saves and recalls data or display image (page116).												






Rear Panel Overview

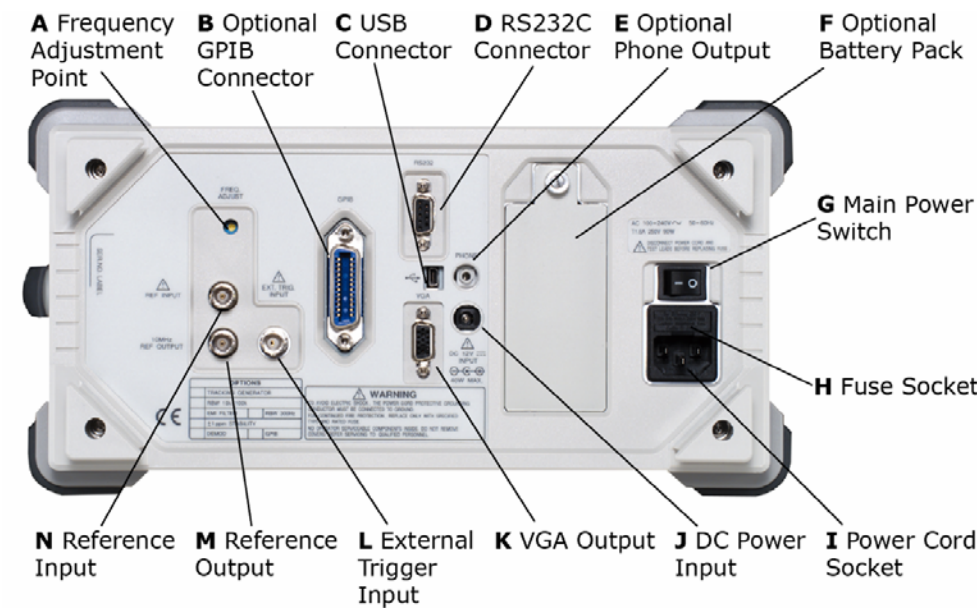


A	Frequency Adjustment Point		Adjusts the internal reference signal frequency; for service operation only.
B	GPIB Connector (Optional)		Optional 24 pin female GPIB connector for remote control (page161). For interface setting details, see page130.
C	USB Connector		Type B mini connector for PC software connection (page153) and remote control (page161). For interface setting details, see page129.
D	RS232C Connector		9 pin female connector for PC software connection (page153) and remote control (page161). For interface setting details, see page129.

E	Phone Output (Optional)		3.5mm phone jack for audio output. Available when the optional Demodulator is installed. For details, see page147.
F	Battery Pack (Optional)		Optional battery pack for portable usage. Installed together with DC operation module. For details, see page151.
G	Main Power Switch		The main switch for turning On/Off the power. For Power up sequence, see page22.
H	Fuse Socket		Stores T1.6A 250V rating fuse. For fuse related safety instructions, see page8.
I	Power Cord Socket		Accepts the AC power cord, 100~240V, 50/60Hz rating. For power related safety instructions, see page8.
J	DC Power Input		Optional power input, DC 12V, 40W max rating. Installed together with the battery pack. For details, see page152.
K	VGA Output		15pin, female VGA connector that outputs 640 x 480 resolution display image to an external monitor. For details, see page114.

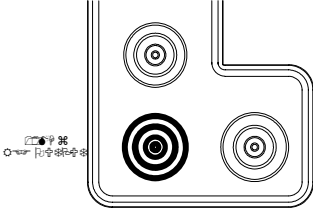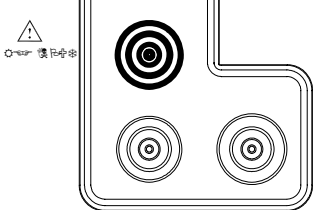L	External Trigger Input		Accepts a trigger signal from an external device. For details, see page106.
M	Reference Output		Outputs +5V TTL, 10MHz reference signal used for synchronizing GSP-830 with external device. For details, see page136.
N	Reference Input		Accepts a signal from an external device, used for synchronization with GSP-830. For details, see page137.



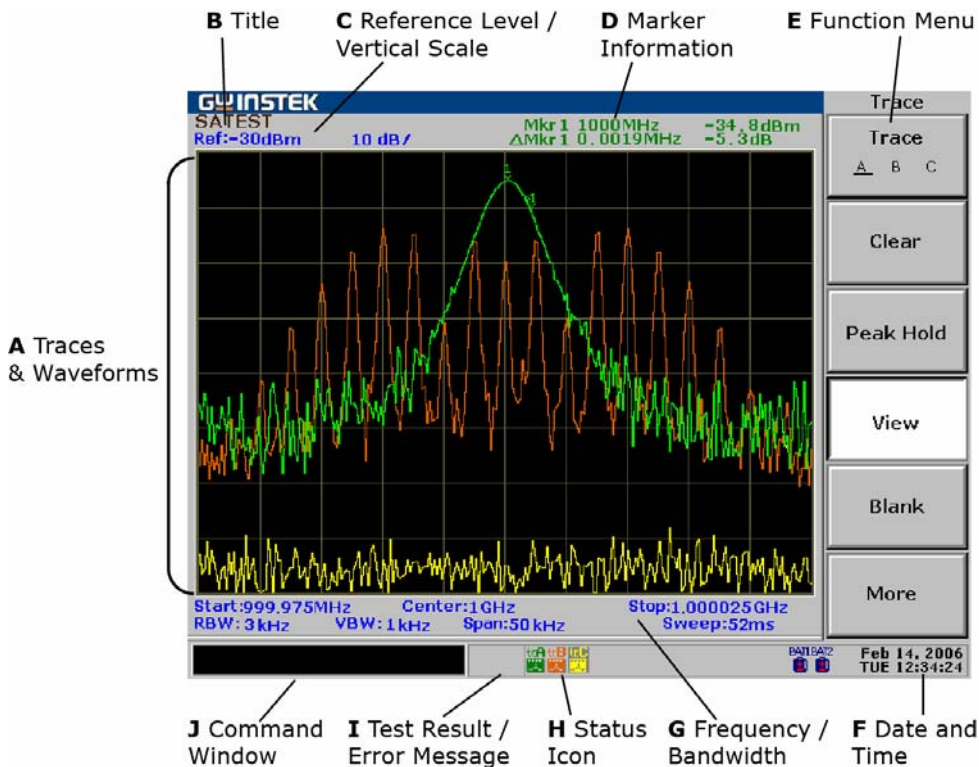



















# Display Overview



A	Traces & Waveforms	Input signal and trace that appears on the main display area. Input signal & TraceA: Green, TraceB: Red, TraceC: Yellow. For trace details, see page75.
B	Title	Title of the current display. For details, see page112.
C	Reference Level/Scale	Reference amplitude level and vertical scale. For amplitude details, see page49.
D	Marker Information	The frequency and amplitude for the active marker / delta marker. For marker details, see page63.
E	Function Menu	The menu associated with F1~F6 function keys on the right side of the display.
F	Date and Time	Current date and time. For setup details, see page135.
G	Frequency/Bandwidth	Upper line: shows the Start/Stop frequency (page45) and the Center frequency (page43). Lower line: shows the Video bandwidth (page101), the Resolution bandwidth (page99), the frequency Span (page43), and the Sweep time (page104).

H	Status Icon	The icons showing various system conditions. See the below Status Icon Overview for details.
I	Test Result/ Error Message	The result of the Pass/Fail test using the Limit lines (page96) or the system error messages (page131).
J	Command Window	Shows the current status of the selected menu or the entered parameters such as frequency and amplitude.



## Status Icon Overview

Amplitude (page49)		External gain On, Amplitude correction On, Input impedance 75Ω, Input impedance calibration On
Peak Search (page70)		Peak Track On
Trace (page75)	 TraceA:green,  B:red,  C:yellow	
		Clear mode
		Average On
		Peak Hold mode
		View mode, Trace math
BW (page98)		RBW, VBW manual mode
		Sweep time manual mode
Trigger (page106)		Video trigger mode
		External trigger signal On
Battery level (page151)		Fully charged
		50% ~ 25%
		75% ~ 50%
		Less than 25%
Options		TG normalization activated (page145)
		External Reference Signal used (page136)
		±1ppm Stability module installed (page136)
Sequence(page139)		Sequence currently running
USB		USB flash drive is detected (page117), or USB remote control connection is detected (page162)



## Tilt Stand & Power Up

### Tilt stand

#### Low angle

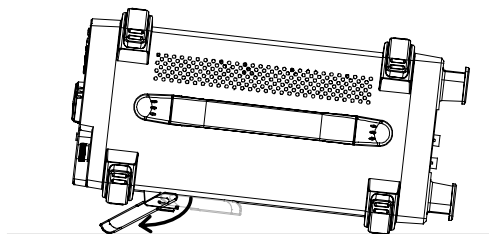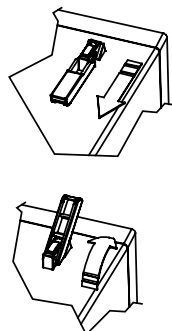


#### High angle

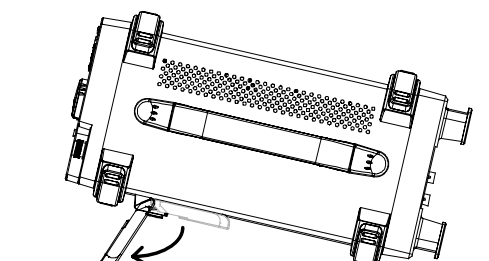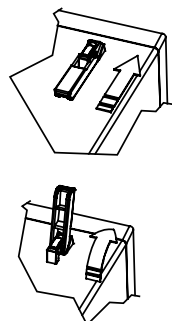


### Power Up

1. Connect the Power cord to the rear panel socket.



2. Turn On the Main power switch.



3. The ON/STBY key on the front panel turns red.



4. Press the ON/STBY key. Its color turns green and the display becomes active.







# Error Check

- This section assumes that GSP-830 is already powered up (page22).

1. Check system error Check the bottom of the display, next to the command window, to see if there is any error message.



Contact the service center if any of the following messages appears.

	External reference input is not working properly.
	Internal reference signal is not working properly.
	Local oscillator 1 is not working properly.
	Local oscillator 3 is not working properly.

2. Check self test result View GSP-830’s self-diagnosis test result. Press the System key→F6 (More) →F2 (Self Test).



The test automatically runs at each power-up. The underline shows the result, Pass or Fail. Contact the service center if any of the items fails.

<div><div>GPIB</div><div><u>Pass</u> Fail</div></div>	<div>F 1</div>	GPIB module connectivity (available only when installed)
<div><div>Flash</div><div><u>Pass</u> Fail</div></div>	<div>F 2</div>	Internal Flash memory for storing the system code/data
<div><div>SDRAM</div><div><u>Pass</u> Fail</div></div>	<div>F 3</div>	Internal SDRAM for running the system code
<div><div>RTC</div><div><u>Pass</u> Fail</div></div>	<div>F 4</div>	Internal real time clock for configuring the date and time

## Functionality Check


- This section assumes GSP-830 is already powered up (page 22).
- Before operating GSP-830 in a new environment, run these steps to make sure it is functionally stable.

### 1. Feed a signal

Input a signal to check if GSP-830 correctly shows the waveform on the display. There are two ways to feed an input signal.


#### Feed the DUT signal

If the Device Under Test is already available, connect the output signal to the RF input terminal. The signal amplitude must be less than +30dBm.

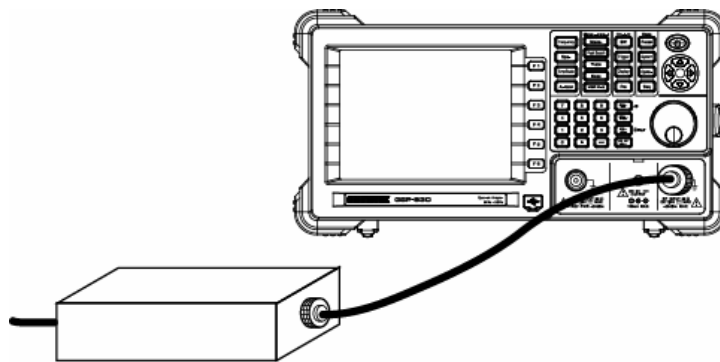

#### Feed the internal auxiliary signal

You can also use the internal auxiliary signal, 100MHz/-30dBm. No cable connection is required in this case. Activate the signal by pressing the System key → F4 (Aux Sig On).





### 2. View signal

Press the AutoSet key → F1 (AutoSet).




GSP-830 automatically configures the horizontal and vertical scales and shows the signal.



Check the peak frequency and amplitude that appear on the top right corner of the display. To move the marker, use the Scroll knob  or Left/Right key .

Internal auxiliary signal, -30dBm @100MHz

Peak frequency/amplitude

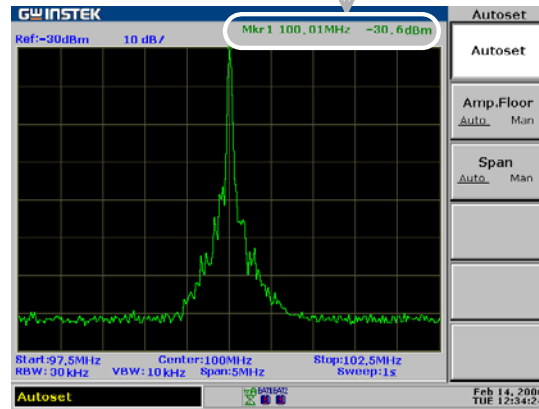

If the displayed value does not match the actual signal, contact the service center.

# QUICK REFERENCE

This chapter collects all the key sequences for panel operations, the menu contents on the display, and the factory installed setting recalled by the Preset key. Use this chapter as a handy reference when you need quick access to the intended operation, and when you need to get an overview of GSP-830 functionalities.

Shortcut	Operation Shortcuts.....	27
Menu Tree	Frequency, Span, Autoset, Amplitude(1 of 2).....	33
	Amplitude (2 of 2), Marker.....	34
	Peak Search, Trace.....	35
	Measurement, Limit Line.....	36
	BW, Trigger, Display.....	37
	File.....	38
	System.....	39
	Option, Sequence.....	40
Preset	Preset Contents.....	41

## Operation Shortcuts

Here is the list of operations introduced in this manual and their shortcuts.

### Frequency and Span

Set Center Frequency and Span	Frequency→F1, Span→F1
Set Start and Stop Frequency	Frequency→F2, F3
Set Frequency Step	Frequency→F4
Activate Full Span (3.0GHz)	Span→F2
Activate Zero Span (Time Domain)	Span→F3
Recall Last Span	Span→F4

### Amplitude

Set Reference Level	Amplitude→F1
Select Vertical Scale	Amplitude→F2
Select Unit (dBm/dBmV/dBuV)	Amplitude→F3→F1~F3
Set External Offset	Amplitude→F4
Activate Amplitude Correction	Amplitude→F5→F2
Select Amplitude Correction Set	Amplitude→F5→F1→F1
Delete Amplitude Correction Item	Amplitude→F5→F1→F2
Delete Amplitude Correction Set	Amplitude→F5→F1→F3→F1, F2
Undo Correction Item/Set Deletion	Amplitude→F5→F1→F4
Save Amplitude Correction Set	Amplitude→F5→F1→F5
Select Input Impedance (50Ω/75Ω)	Amplitude→F6→F1
Set Input Impedance Offset	Amplitude→F6→F2

### Autoset

Run Autoset	Autoset→F1
Set Amplitude Floor	Autoset→F2
Set Frequency View Span	Autoset→F3

## Marker

Activate Normal Marker	Marker→F1, F2
Activate Delta Marker	Marker→F1, F2, F3
Activate All Normal Markers	Marker→F6→F3
Move Marker to Peak	Marker→F4 or Peak Search→F1
Move Marker and Peak to Center	Marker→F4, F5 or Peak Search→F5
Track Marker on Peak	Peak Search→F6→F4
Move Marker to Various Locations	Marker→F6→F4→F1~F5
Show Marker Table	Marker→F6→F2
Put Marker on Trace	Marker→F6→F1

## Peak Search

Search Peak Signal	Peak Search→F1 or Marker→F4
Search Next Peak	Peak Search→F2, F3 (right), F4 (left)
Search Peak and Move to Center	Peak Search→F5 or Marker→F4, F5
Track Marker on Peak	Peak Search→F6→F4
Search Minimum Amplitude	Peak Search→F6→F5
Show Peak Table	Peak Search→F6→F1
Sort Peaks in Peak Table	Peak Search→F6→F2
Set Peak Threshold	Peak Search→F6→F3

## Trace

Activate Trace	Trace→F1
Update Trace in Real-Time (Default)	Trace→F2
View Peak Hold Trace	Trace→F3
Freeze Trace	Trace→F4
Hide Trace	Trace→F5
View Averaged Trace	Trace→F6→F1 or BW→F4
Run Trace Math	Trace→F6→F2→F1~F5
Select Signal Detection Mode	Trace→F6→F3→F1~F5

## Power Measurement

Activate ACPR	Meas→F2
Set ACPR Main Channel Bandwidth	Meas→F1→F1
Set ACPR Channel Space	Meas→F1→F2
Set Adjacent Channel Offset	Meas→F1→F4→F2, F4
Set Adjacent Channel Bandwidth	Meas→F1→F4→F1, F3
Move ACPR Channel Up	Meas→F4
Move ACPR Channel Down	Meas→F5
Activate OCBW	Meas→F3
Set OCBW Channel Bandwidth	Meas→F1→F1
Set OCBW Channel Space	Meas→F1→F2
Set OCBW %	Meas→F1→F3
Move OCBW Channel Up	Meas→F4
Move OCBW Channel Down	Meas→F5
Activate N dB	Meas→F6→F1
Set N dB Value	Meas→F6→F2
Activate Phase Jitter	Meas→F6→F3
Set Phase Jitter Offset	Meas→F6→F4→F1(Start), F2(Stop)

## Limit Line

Activate Limit Line	Limit Line→F1 (High), F2 (Low)
Select Limit Line for Edit	Limit Line→F3→F1
Activate Limit Line Edit Table	Limit Line→F3→F2
Delete Limit Line Table Item	Limit Line→F3→F3 (Delete)
Delete All Table Item	Limit Line→F3→F4→F1, F2
Undo Last Deletion	Limit Line→F3→F5
Run Pass/Fail Test	Limit Line→F4
Select Pass/Fail Condition	Limit Line→F5

## Bandwidth

Select RBW	BW→F1
Select VBW	BW→F2
Set Sweep Time	BW→F3
Set Trace Average Number	BW→F4 or Trace→F6→F1
Reset RBW/VBW/Sweep to Auto	BW→F5

## Trigger

Select Free Run (Default)	Trigger→F1
Select Video/External Trigger	Trigger→F2
Select Trigger Mode	Trigger→F3
Set Trigger Delay	Trigger→F4
Set Trigger Frequency	Trigger→F5
Run Trigger (in Single/Continuous)	Trigger→F6

## Display

Change Dimmer Level	Display→F1
Show Display Line	Display→F2
Clear Title	Display→F3→F1
Enter Title	Display→F3→F2~F4
Show Title	Display→F3→F5
Activate Split Display	Display→F4→F1 (Upper), F2 (Lower)
Alternate Upper/Lower Sweep	Display→F4→F3
Switch Split Display to Full Screen	Display→F4→F4

## File

Select Copy Source File	File→F1→F1→F1~F5
Select Copy Destination File	File→F1→F2→F1~F5
Edit Copied File Name	File→F1→F3

Copy Selected File	File→F1→F4
Select File for Deletion	File→F2→F1→F1~F5
Delete Selected File	File→F2→F2
Rename File	File→F3→F1
Confirm New File Name	File→F3→F2
Save Display Image to USB Drive	File→F4→F1→F2
Rename File in USB Drive	File→F4→F1→F1

## Preset

Recall Preset Panel Setting	Preset
-----------------------------	--------

## System

Save Setup	System→F1→F1~F2 (Select), F3 (Save)
Recall Setup	System→F1→F1~F2(Select),F4(Recall)
Set GPIB Address	System→F2
Show RS-232C Configuration	System→F3→F1~F4
Activate Auxiliary Signal	System→F4
Set Date	System→F6→F1→F1→F1~F4
Set Time	System→F6→F1→F2→F1~F3
Activate Clock Display	System→F6→F1→F3
View Self Test Result	System→F6→F2→F1~F4
View System Configuration	System→F6→F4
Select Language	System→F6→F5→F1

## Option

Activate Tracking Generator	Option→F1→F1
Set Tracking Generator Amplitude	Option→F1→F2
Normalize Tracking Generator	Option→F1→F3→F1 (No), F2 (Yes)
Activate Normalized TG	Option→F1→F4
Set Ref Level for TG Normalization	Option→F1→F5

Activate FM Demodulator	Option→F2→F1
Activate AM Demodulator	Option→F2→F2
Activate Phone Output	Option→F2→F3
Set Phone Output Volume	Option→F2→F4
Set Squelch Level	Option→F2→F5
View Battery Level	Option→F3
Set Ext. Reference Signal Frequency	Option→F4

## Sequence


Select Sequence Set	Sequence→F1, F2
Start Sequence Edit	Sequence→F3→F1
Insert 100ms Delay	Sequence→F3→F2
Insert Pause in Sequence	Sequence→F3→F3
Insert Another Sequence Set	Sequence→F3→F4→F1~F2
Stop Sequence Edit	Sequence→F3→F5
Insert Item to Sequence Set	Sequence→F3→F6→F1
Save Sequence Set	Sequence→F3→F6→F2
Delete Sequence Item	Sequence→F3→F6→F3
Delete Sequence Set	Sequence→F3→F6→F4→F1, F2
Undo Sequence Item/Set Delete	Sequence→F3→F6→F5
Select Sequence Run Mode	Sequence→F4→F1
Run Sequence	Sequence→F4→F2
Delete All Sequence Set	Sequence→F5→F1 (No), F2 (Yes)






## Amplitude (2 of 2), Marker


## Amplitude

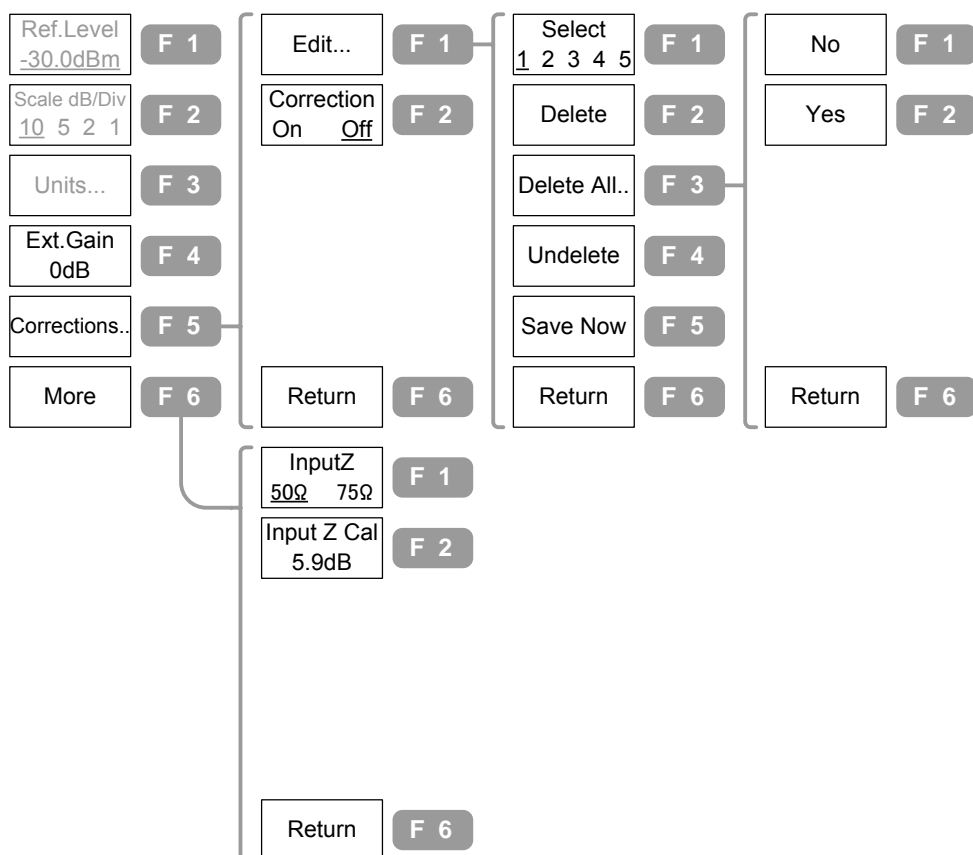



## Marker

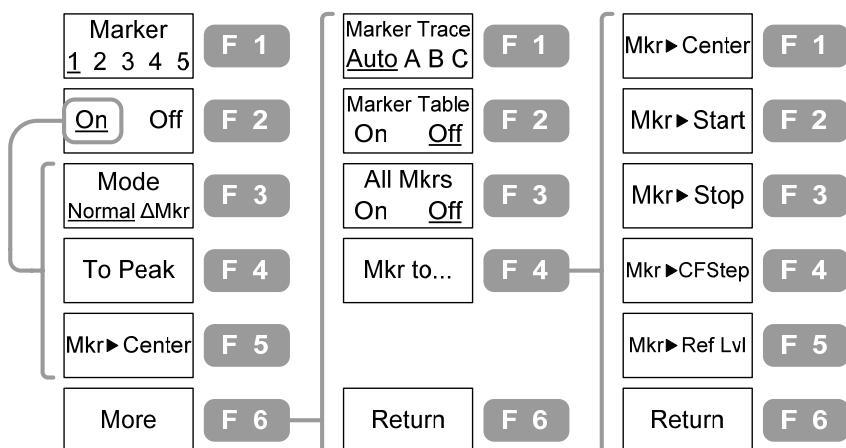


Peak Search, Trace

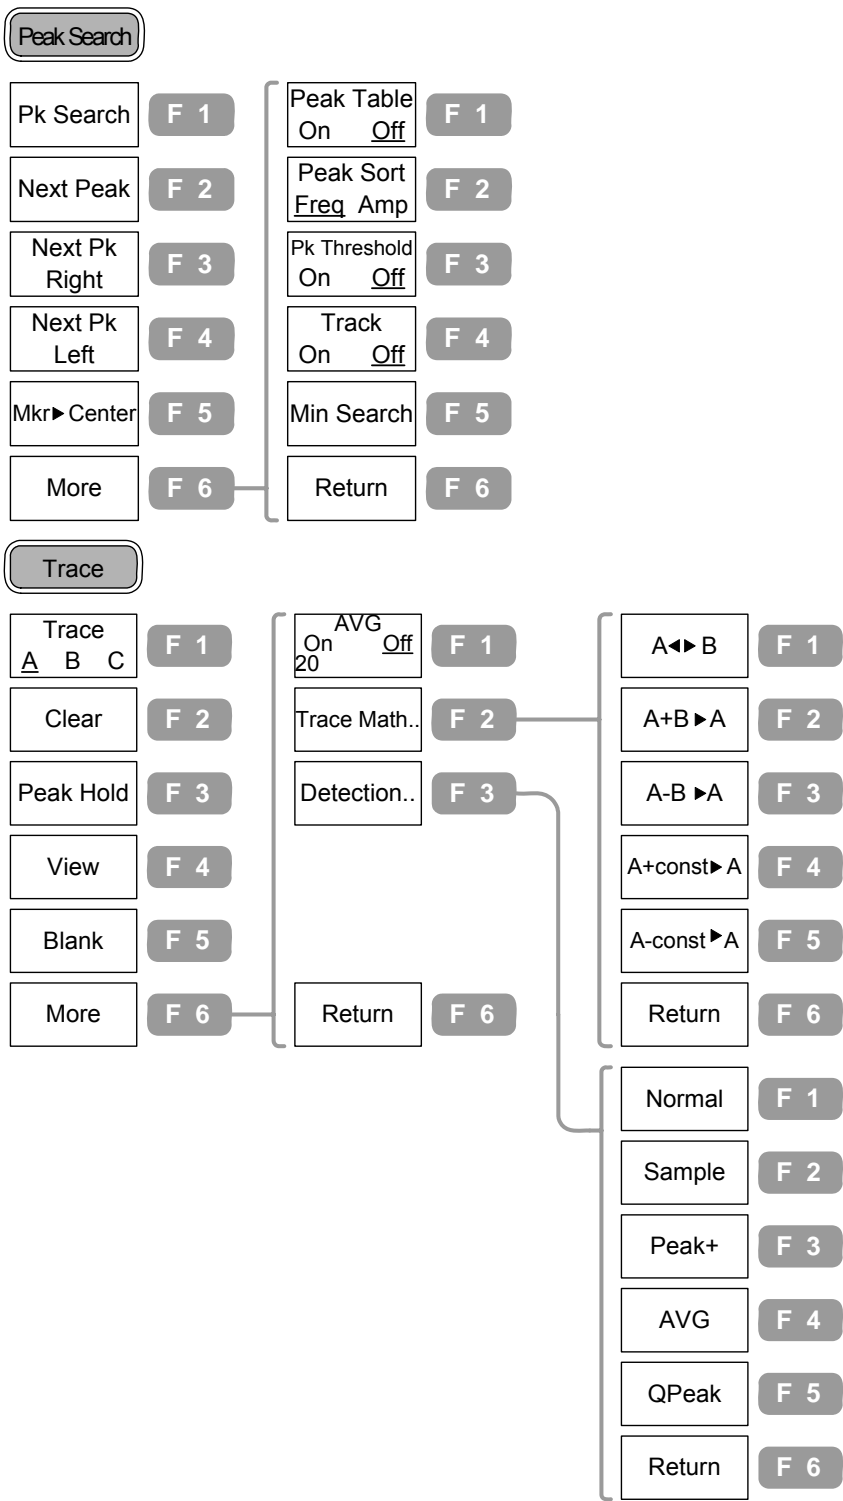


## Measurement, Limit Line

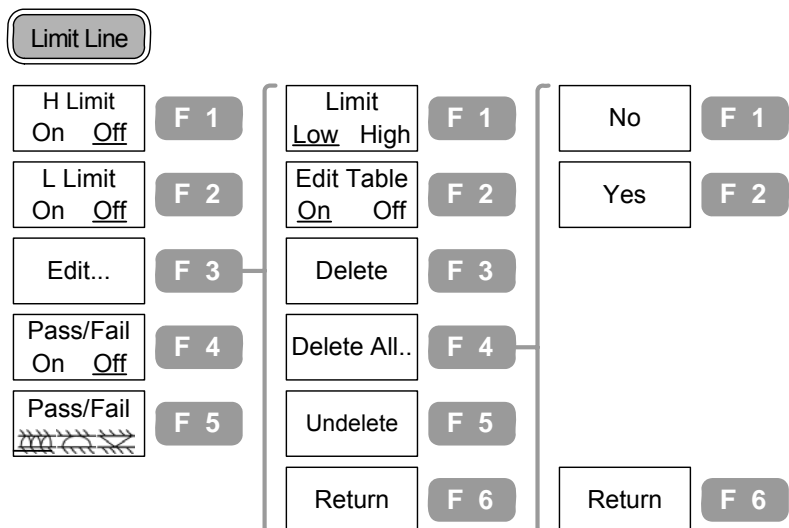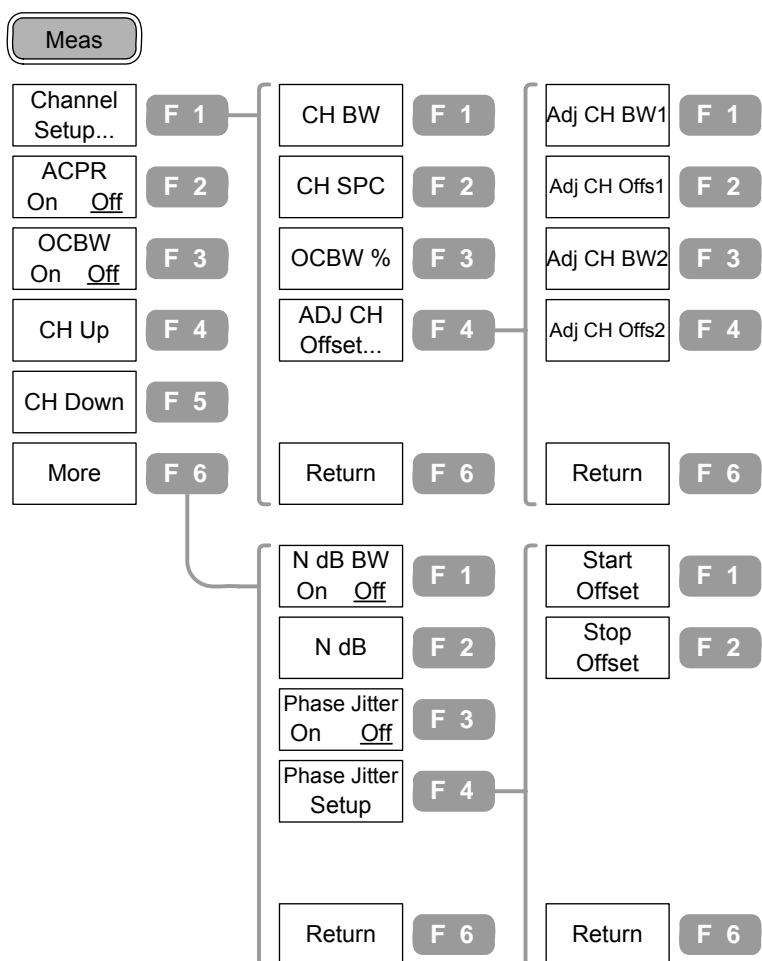


BW, Trigger, Display

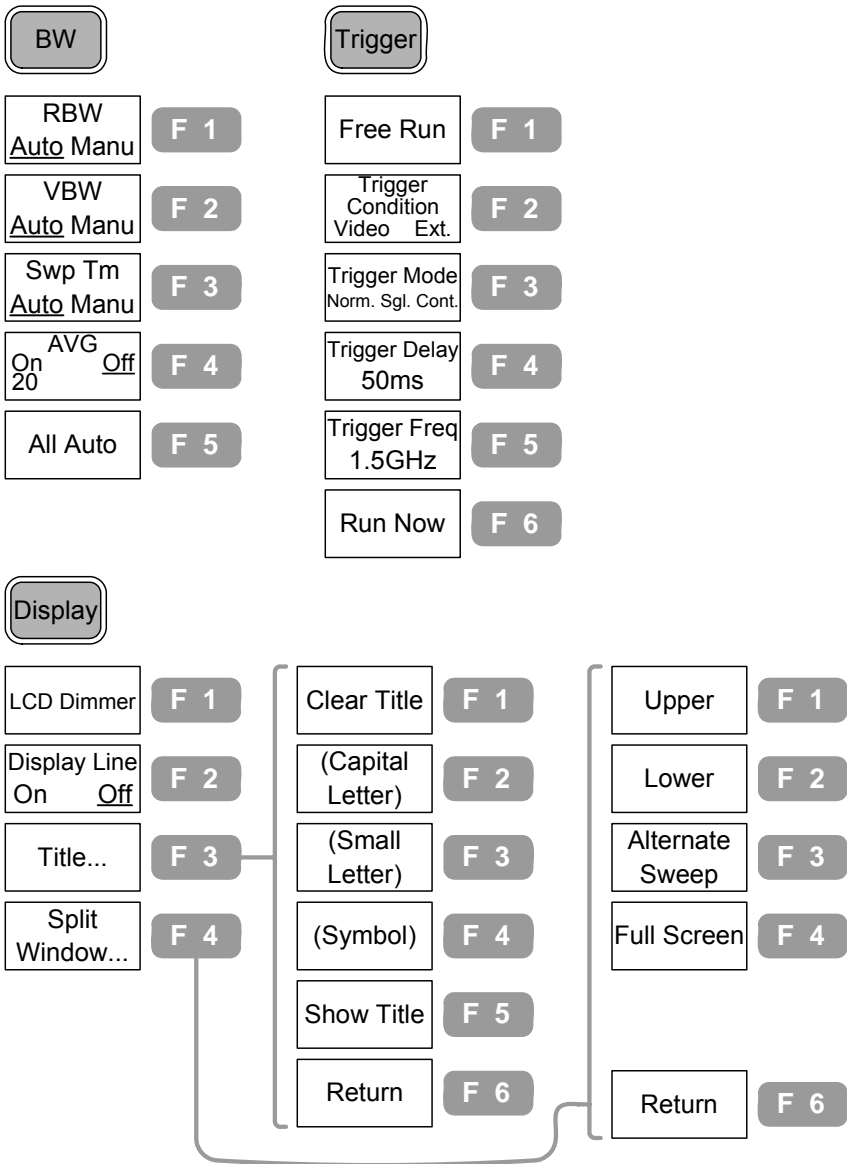

## File

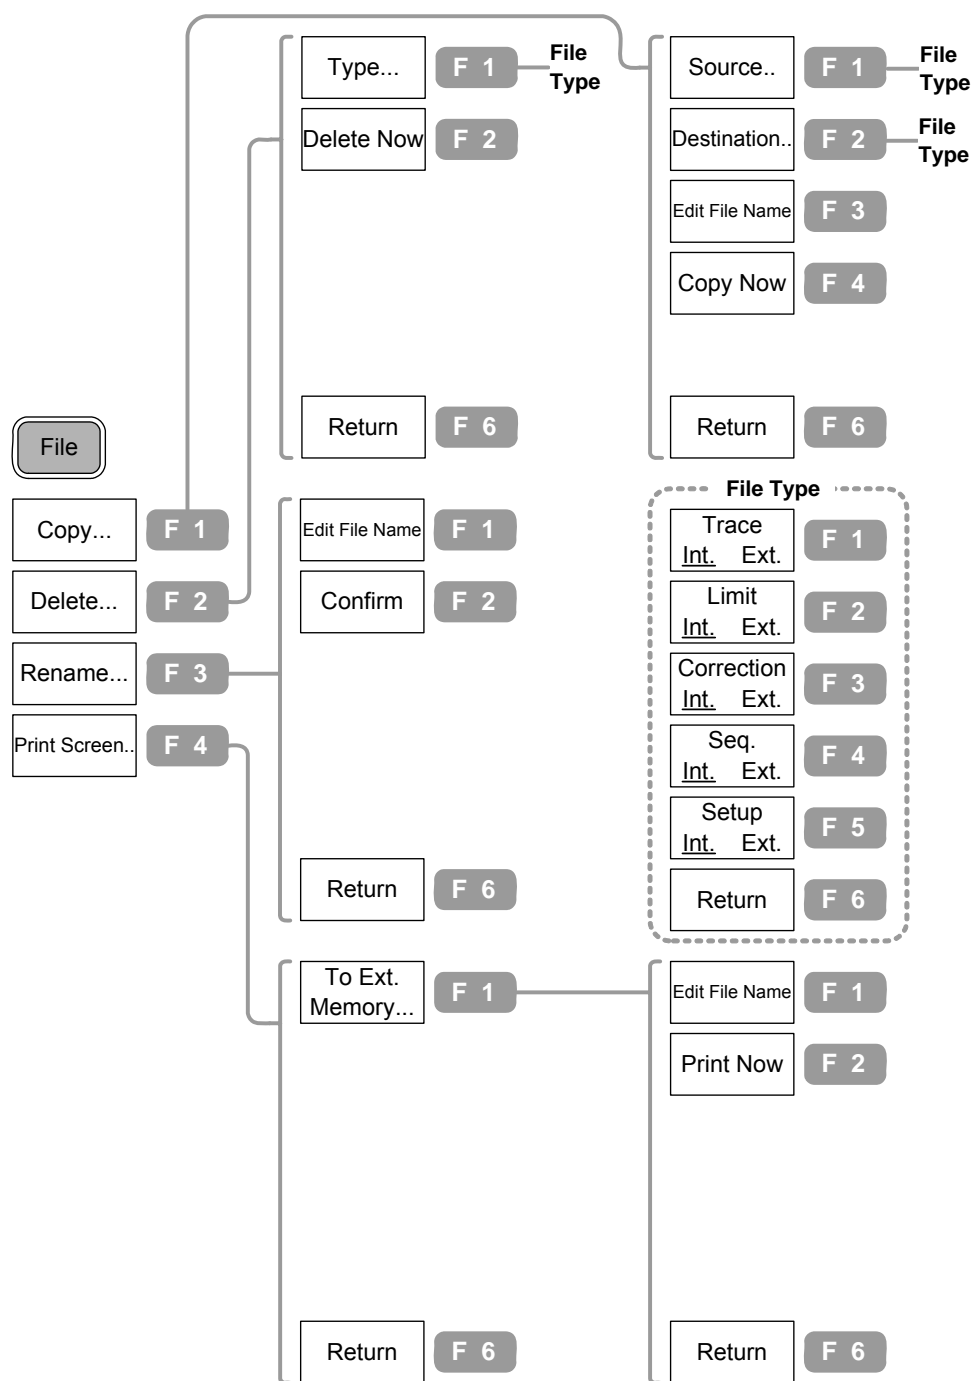


System

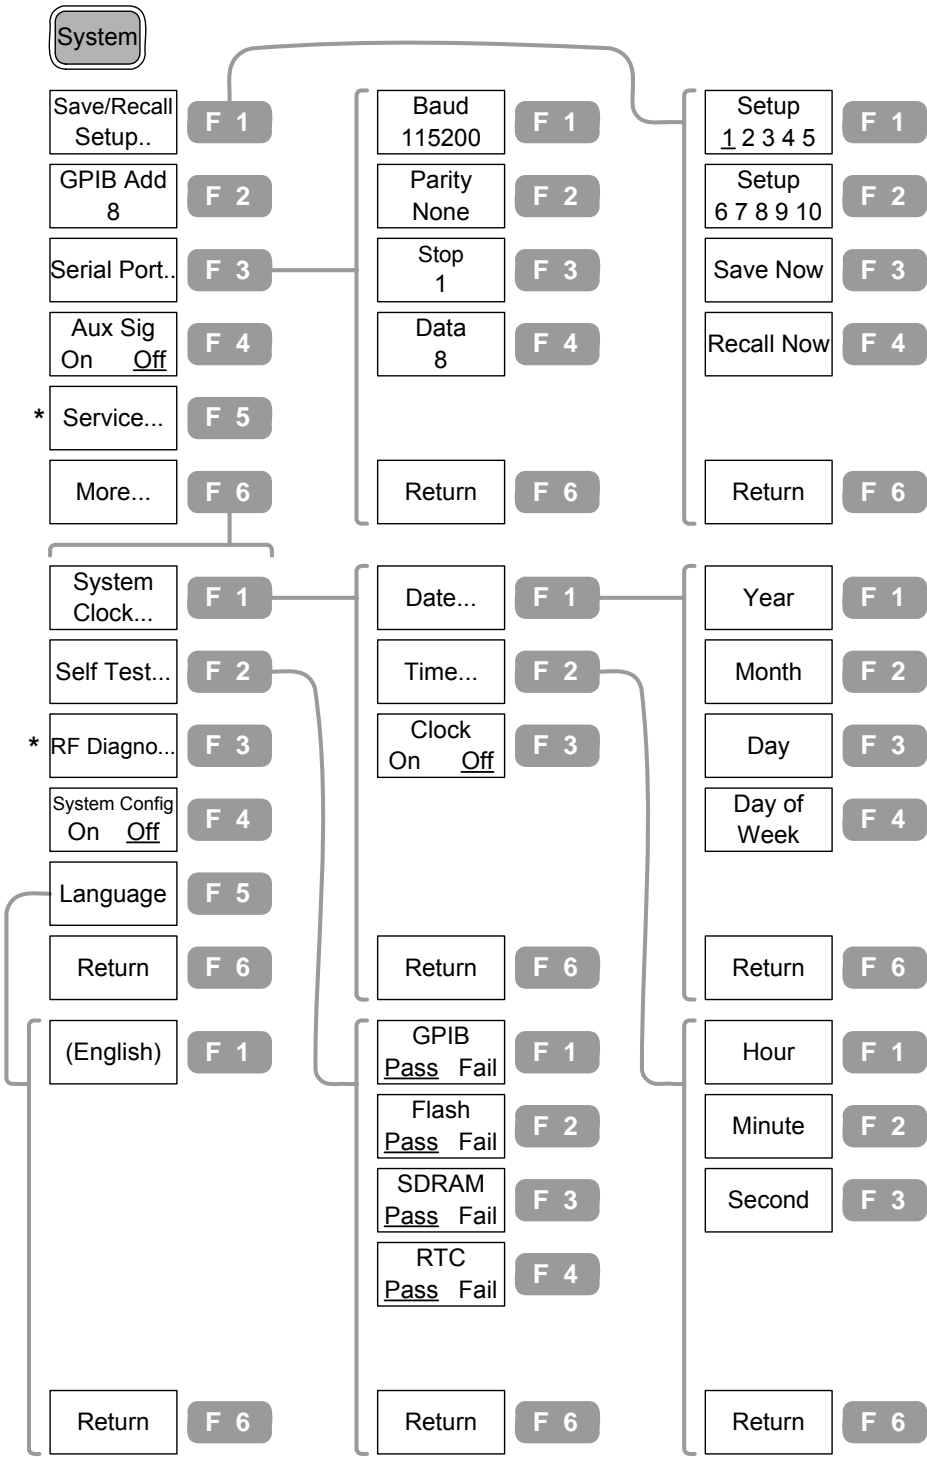


\* Submenu only for service personnel

## Option, Sequence

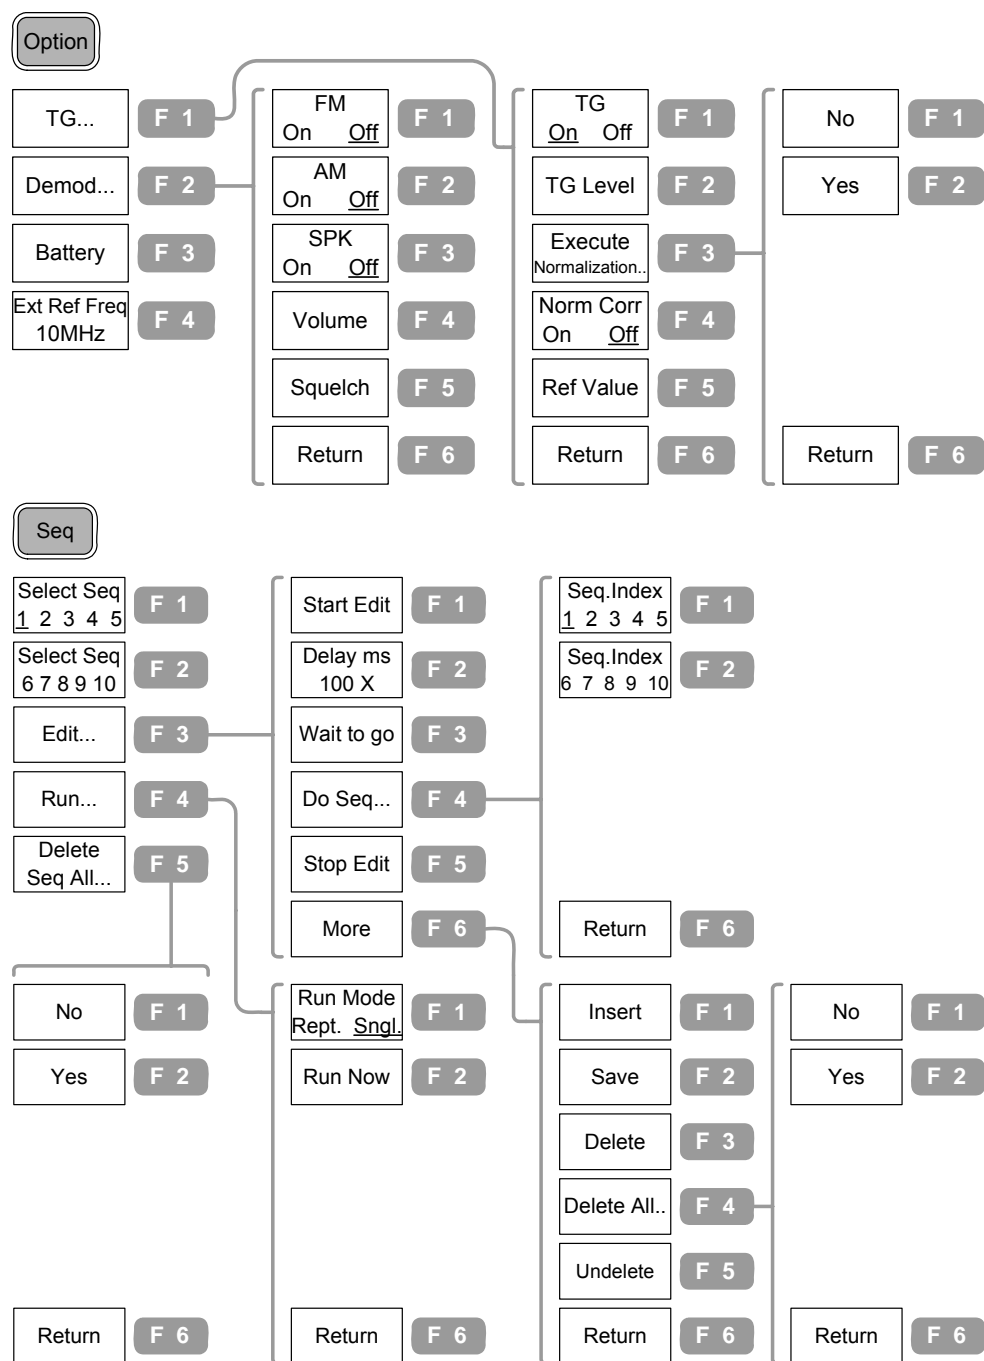




## Preset Contents

These are the settings that appear when pressing the Preset key .

Frequency	Center: 1.5GHz Start: 0Hz	Stop: 3GHz Step: 1MHz
Span	3GHz	
Amplitude	Ref.level: 0dBm Unit: dBm Correction: Off	Scale: 10dB/ External Gain: 0dB Input Z: 50Ω
Autoset	Amplitude Floor: Auto	Span: Auto
Marker	Marker: Off Marker Table: Off	Marker Trace: Auto All Marker: Off
Peak Search	Peak Table: Off Peak Threshold: Off	Peak Sort: Freq Peak Track: Off
Trace	Trace: A AVG: Off	Mode: Clear Detection: Normal
Meas	ACPR: Off CH SPC: 0 CH BW: 600MHz OCBW %: 0 N dB: Off	OCBW: Off Adj CH Offs1: 600MHz Adj CH Offs2: 1200MHz Adj CH BW1&2: 600MHz Phase Jitter: Off
Limit Line	H & L Limit: Off	Pass/ Fail: Off
BW	RBW: Auto SwpTime: Auto	VBW: Auto Average: Off
Trigger	Trigger Delay: 50ms Trigger Mode: Normal	Trigger Freq: 1.5GHz
Display	LCD Dimmer: 5 Split Window Lower: Off	Display Line: Off Split Window Upper: Off
File	Copy Type: Int. Trace Rename Type: Ext. Trace	Delete Type: Int. Trace
System	GPIB Add: 2 Aux Sig: Off	System Config: Off Language: English
Option	External Ref Freq: 10MHz TG Norm Corr: Off Demod AM: Off	TG Output: Off TG Ref Value: 0dBm Demod FM: Off
Sequence	Sequence: 1	Run Mode: Single

# FREQUENCY/SPAN

**Frequency** key, together with **Span** key, sets the frequency scale. Two methods are available. Center-and-Span method defines the center point and the surrounding frequency range. Start-and-Stop method defines the beginning and the end of the frequency range. Special span settings are available at full/zero span. You can also recall the last span setting.

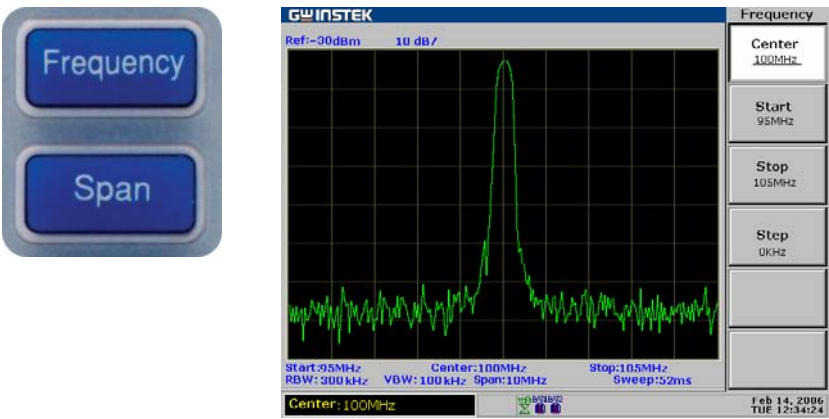






Center and Span	Set frequency adjustment step .....	43
	Set Center Frequency.....	43
	Set Frequency Span.....	44
Start and Stop	Set frequency adjustment Step .....	45
	Set Start frequency.....	45
	Set Stop frequency.....	46
Span	Display Full Frequency Span (3.0GHz) .....	47
	Display Zero Span (time domain view).....	47
	Recall the Last Span Setting.....	48




### View Signal (Center and Span)

Center-and-Span method defines the Center frequency and the left/right bandwidth (Span) to locate the signal.


## Set frequency adjustment step

Background	Frequency adjustment step defines the Arrow key resolution for Center, Start, and Stop frequency.	
Panel operation	<ol style="list-style-type: none"> <li>Press the Frequency key.</li> <li>Press F4 (Step).</li> <li>Enter the value using the numerical keys, Arrow key, and Scroll knob.</li> </ol>	   
Range	<p>0.0kHz ~ 3.0GHz</p> <p>* Arrow key and Scroll knob resolution: 1/10 of Span</p>	

## Set Center Frequency

Panel operation	<ol style="list-style-type: none"> <li>Press the Frequency key.  </li> <li>Press F1 (Center).  </li> <li>Enter the value using the numerical keys, Arrow key, and Scroll knob.  </li> </ol>
Range	<p>0.0kHz ~ 3.0GHz</p> <p>Arrow key and Scroll knob resolution: step value</p>
Note	<ul style="list-style-type: none"> <li>Center frequency/span automatically changes according to start/stop frequencies setting, and vice versa.</li> </ul>


Display

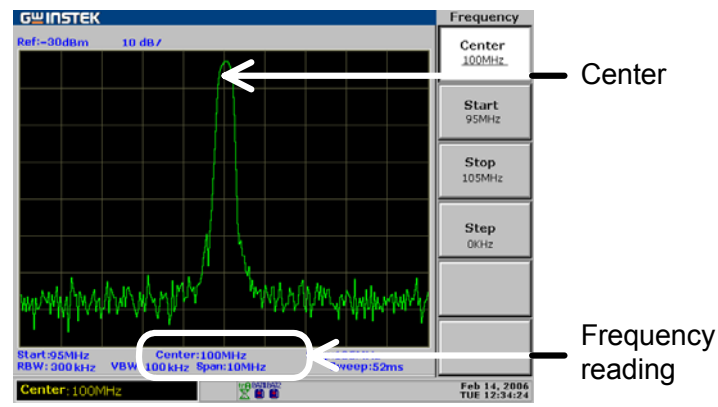


## Set Frequency Span

Panel operation

1. Press the Span key.



2. Press F1 (Span).



3. Enter the value using the numerical keys, Arrow key, and Scroll knob.




Range

2kHz ~ 3GHz

\* Arrow key & Scroll knob resolution: 1-2-5 sequence  
(0 [zero span], 2kHz, 5kHz, 10kHz, 20kHz, 50kHz, ....1GHz, 2GHz, 3GHz)

Display

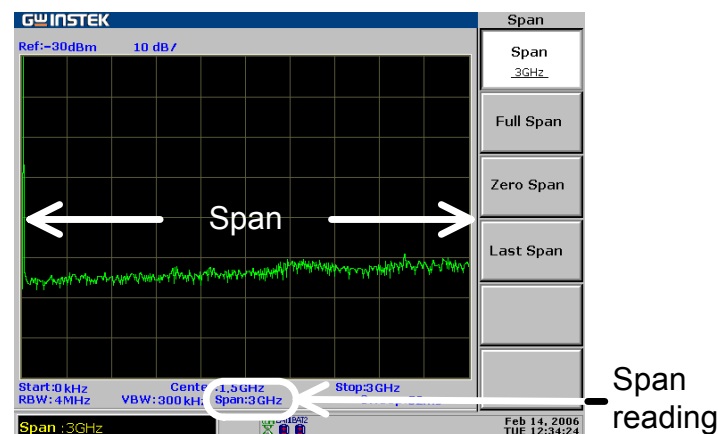





Note

- Center frequency/span automatically changes according to start/stop frequency settings, and vice versa.




### View Signal (Start and Stop)

Start-and-Stop method defines the beginning (Start) and the end (Stop) of the frequency range.


### Set frequency adjustment Step

Background	Frequency adjustment step defines the Arrow key resolution for Center, Start, and Stop frequency.	
Panel operation	<ol style="list-style-type: none"> <li>Press the Frequency key.</li> <li>Press F4 (Step).</li> <li>Enter the value using the numerical keys, Arrow key, and Scroll knob.</li> </ol>	  
Range	0.0kHz ~ 3.0GHz * Arrow key and Scroll knob resolution: 1/10 of Span	

## Set Start frequency

Panel operation	
1. Press the Frequency key.	
2. Press F2 (Start).	
3. Enter the value using the numerical keys, Arrow key, and Scroll knob.	
Range	0.0kHz ~ 3.0GHz (Start Frequency ≤ Stop Frequency) Arrow key and Scroll knob resolution: Step value
Note	<ul style="list-style-type: none"> <li>Center frequency/span automatically change according to start/stop frequency settings, and vice versa.</li> </ul>

Display

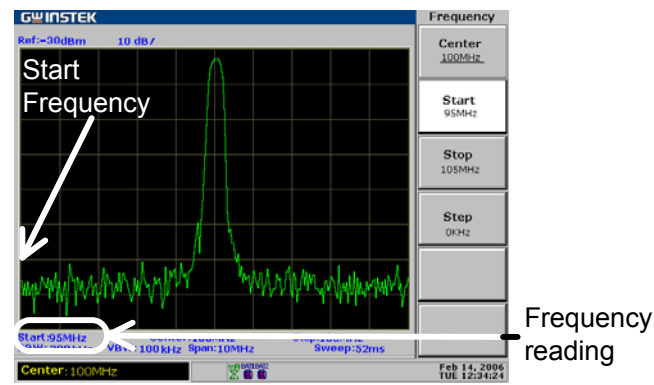


## Set Stop frequency

Panel operation

1. Press the Frequency key.



2. Press F3 (Stop).



3. Enter the value using the numerical keys, Arrow key, and Scroll knob.




Range

0.0kHz ~ 3.0GHz (Start Frequency ≤ Stop Frequency)

\* Arrow key resolution: Step value

\* Scroll knob resolution: 1/500 of Span

Display

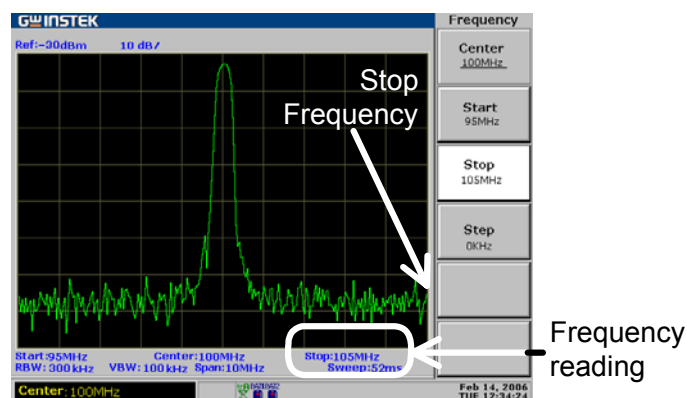

Note


- Center frequency/span automatically change according to start/stop frequency settings, and vice versa.

## Full/Zero Span

Full or Zero Span sets the span to extreme values: 3.0GHz (full) or 0kHz (zero). They provide faster ways to view signals in certain situations, such as in time domain (zero span) for viewing modulation or in full span for viewing frequency unknown signal.

### Display Full Frequency Span (3.0GHz)

Panel operation	1. Press the Span key.	<div>Span</div>
	2. Press F2 (Full Span).	<div>Full Span</div> <div>F 2</div>
Range	3.0GHz (fixed) <div>Full span also sets these parameters to fixed values.<ul style="list-style-type: none"><li>Center Frequency: 1.5GHz</li><li>Start frequency: 0.0kHz</li><li>Stop frequency: 3.0GHz</li></ul></div>	

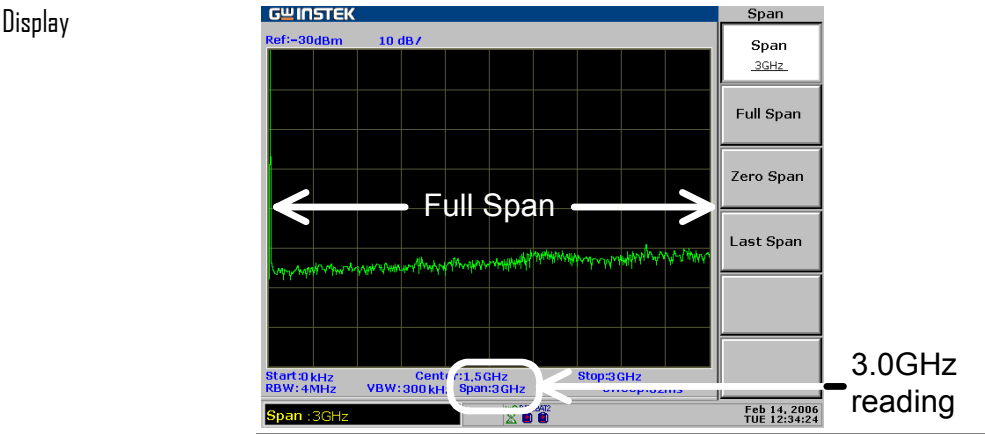


### Display Zero Span (time domain view)

Panel operation	1. Press the Span key.	<div>Span</div>
	2. Press F3 (Zero Span).	<div>Zero Span</div> <div>F 3</div>
Range	Center frequency (fixed)	




- Zero span also sets these parameters to fixed values.
- Start frequency: same as the Center frequency
  - Stop frequency: same as the Center frequency

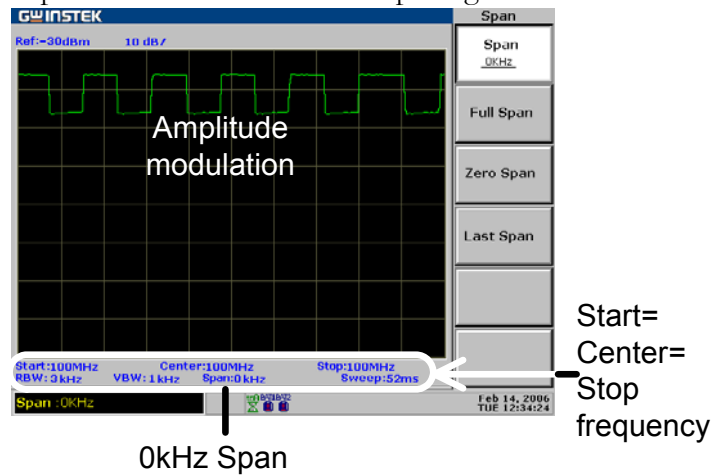Display                   The diagram shows an example of observing the amplitude modulation of the input signal.



- Note
- Make sure the RBW setting is large enough when using Zero Span for viewing amplitude modulation. For RBW setting details, see page99.

## Recall the Last Span Setting

- Panel operation
1. Press the Span key. 
  2. Press F4 (Last Span).  
  3. The span setting goes back to the previous one.


Nesting level           1 level

格式化: 标题 1



# AMPLITUDE

**Amplitude key** sets the vertical scale of the display, including the upper limit (Reference Level), vertical range/unit (Amplitude Scale and Unit), and compensation for external gain or loss (External Offset). Amplitude Correction adjusts the frequency response distortion caused by external networks. Pre-Amplifier is an optional item that boosts the level of weak input signal before entering GSP-830. You can also set input impedance level according to the application needs.

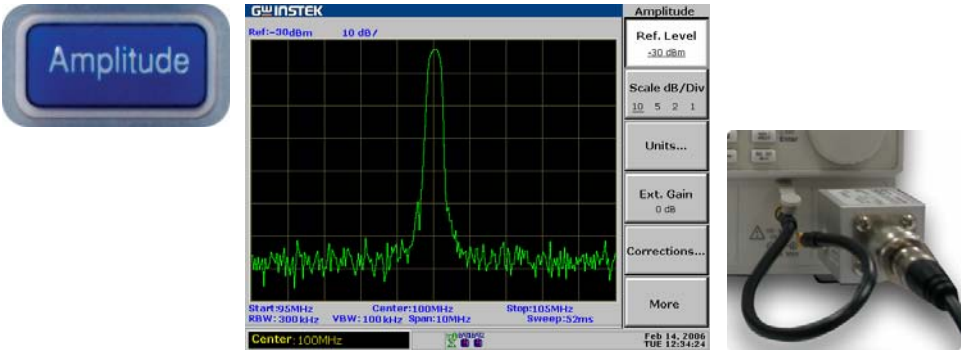




Vertical Scale Setting	Set reference amplitude level.....	50
	Select Amplitude scale .....	51
	Select Amplitude Unit .....	51
	Set External Offset level.....	52
Amplitude Correction	Correct amplitude step by step .....	53
	Delete entire correction set data.....	56
	Recall existing correction set.....	57
	Save/copy/delete/rename correction file .....	57
Pre-Amplifier	Use Pre-Amplifier GAP-801 (Optional).....	58
Input Impedance	Select input impedance (50Ω/75Ω).....	59
	Set impedance offset (75Ω only).....	59


# Set Vertical Scale

Vertical display scale is defined by the reference amplitude level, vertical amplitude range, measurement unit, and external gain/loss setting.


## Set reference amplitude level

The reference level defines the uppermost display level.

Panel operation	1. Press the Amplitude key.	
	2. Press F1 (Ref.Level).	
	3. Enter the value using the numerical keys, Arrow key, and Scroll knob.	
Range	dBm	-110 ~ +20 dBm, 0.1dB resolution
	dBmV	-63.01 ~ +66.99 dBmV, 0.01dB resolution
	dBuV	-3.01 ~ +126.99 dBuV, 0.01dB resolution

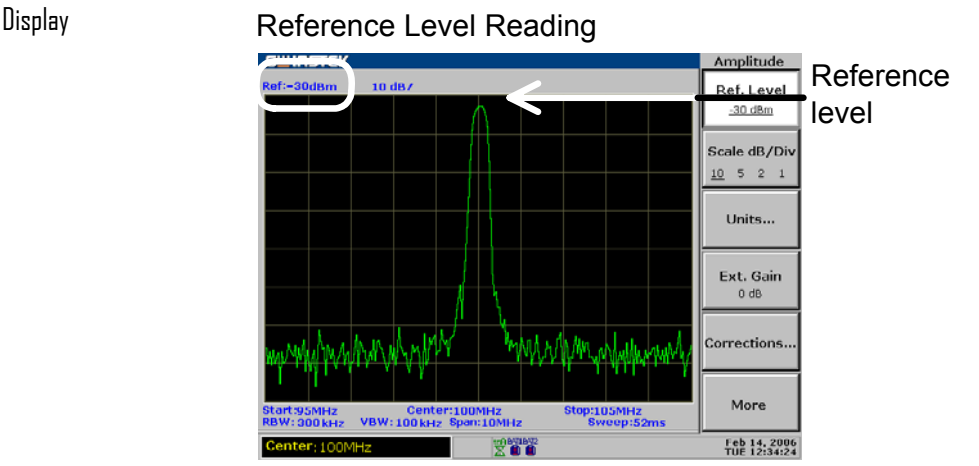




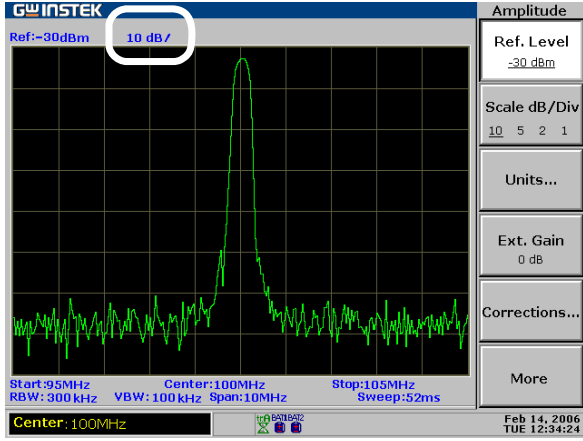
### Select Amplitude scale

Panel operation	1. Press the Amplitude key.	<div>Amplitude</div>
	2. Press F2 (Scale dB/Div) repeatedly to select the scale.	<div>Scale dB/Div</div> <div>10 5 2 1</div> <div>F 2</div>
Range	10, 5, 2, 1 dB/Div	
Display	<div>Scale reading</div> 	


### Select Amplitude Unit

Panel operation	1. Press the Amplitude key.	<div>Amplitude</div>
	2. Press F3 (Units).	<div>Units...</div> <div>F 3</div>
	3. Select and press the unit from F1 (dBm), F2 (dBmV), and F3 (dBuV).	<div>dBm</div> <div>F 1</div> <div>dBmV</div> <div>F 2</div> <div>dBuV</div> <div>F 3</div>
	4. Press F6 (Return) to go back to the previous menu.	<div>Return</div> <div>F 6</div>
Range	dBm	-110 ~ +20 dBm
	dBmV	-63.01 ~ +26.99 dBmV
	dBuV	-3.01 ~ +126.99 dBuV


## Set External Offset level

Background	External offset compensates amplitude gain or loss caused by an external network or device.	
Panel operation	1. Press the Amplitude key.	
	2. Press F4 (Ext.Gain).	
	3. Enter the value using the numerical keys.	
Range	-20.0dB ~ +20.0dB, 0.1dB resolution	
Icon		Amplitude icon appears at the bottom of the display when the external offset level is changed.

Example  
Before (Offset: 0dB)

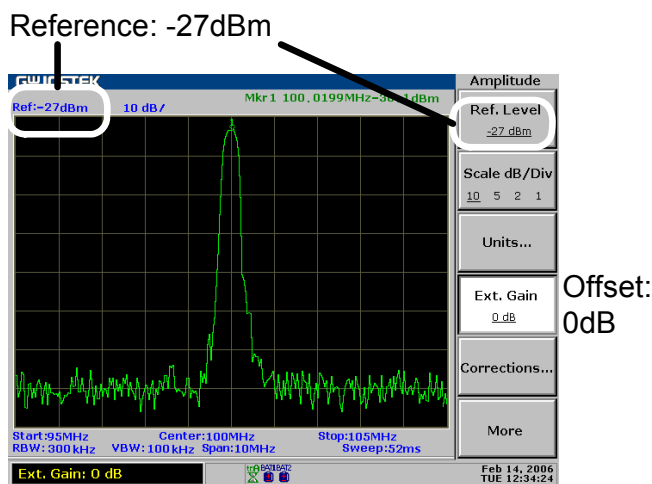

After (Offset: -3dB)

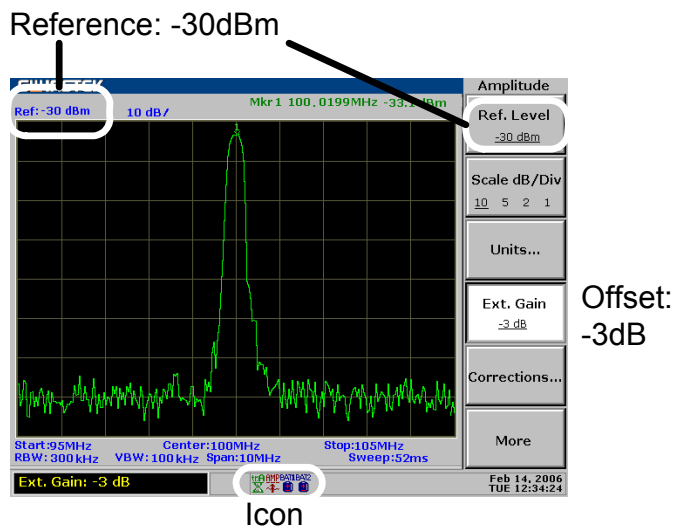


# Amplitude Correction

## Overview

**Background** Amplitude correction adjusts GSP-830's frequency response by changing amplitude for specific frequencies.

**Menu tree**

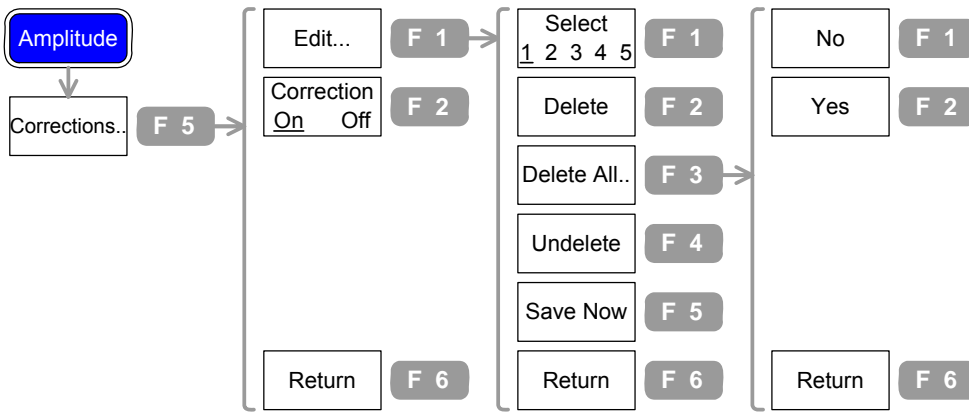


Range	Correction set	5 set, 30 correction points each
	Amplitude	−40 ~ +40dB per correction point, 0.1dB resolution
	Frequency	9kHz ~ 3.0GHz, 1kHz resolution
Icon		Amplitude icon appears at the bottom of the display when amplitude correction is On.

## Correct amplitude step by step

**Example description** In this example, the network between GSP-830 and DUT distorts the waveform and pushes the level down at around 2.4GHz. Amplitude correction can fix the level.


Correction level	In this example the amplitude around 2.4GHz is boosted by +1 ~ +3dB.	
	2.2GHz	+2.5dB
	2.3GHz	+1.3dB
	2.4GHz	+2.8dB
	2.5GHz	+2.5dB
	2.6GHz	+1.2dB

Diagram

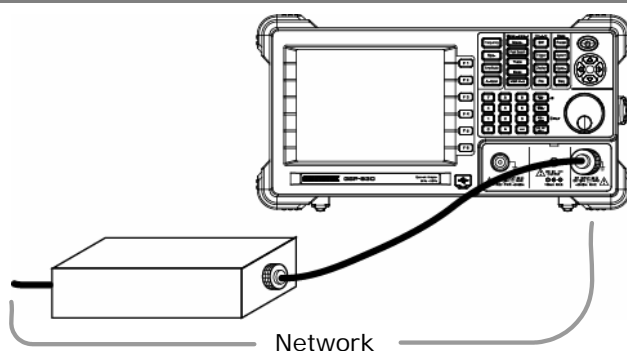

Waveform (before correction)

The frequency response is distorted (non-flat) and the level is attenuated by 2 ~ 3dB.

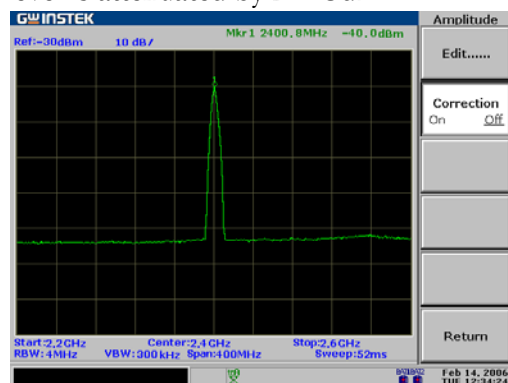


1. Enter correction edit mode



1. Press the Amplitude key.



2. Press F5 (Corrections).



3. Press F1 (Edit). The display shows the correction sets.

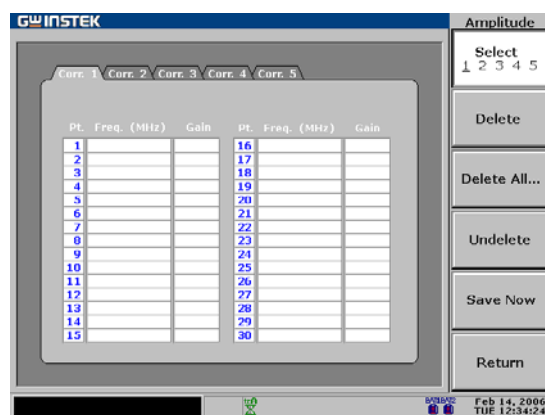

2. Select correction set

Press F1 (Select) repeatedly to select the correction set. 5 sets, 30 points each, are selectable.

Example: correction set 3 selected

Corr. 1

Corr. 2

Corr. 3

Select

1 2 3 4 5

F 1
- 3a. Add correction point

- Make sure that the cursor is pointing to the first empty frequency point.

Pt.

Freq. (MHz)

Gain

1

2

3

4

5

- If necessary, move the cursor using the Up/Down key.
- Enter the frequency in MHz using the numerical keys. 9.0kHz ~ 3.0GHz.

0

1

2

3

4

5

6

7

8

9

DEL

+

Hz

kHz

MHz

GHz
- The cursor automatically moves to the Gain side. Enter the gain in dB using the numerical keys. -40dB ~ +40dB.

Pt.

Freq. (MHz)

Gain

1

2200

2

3

4

5

0

1

2

3

4

5

6

7

8

9

DEL

+

Hz

kHz

MHz

GHz
- Repeat the above procedure for all correction data. The points are automatically sorted by the frequency (low → high).

3b. Modify correction point

- Move the cursor using the Arrow key.
- Enter the new frequency or gain using the numerical keys.

Pt.

Freq. (MHz)

Gain

1

2200

2.5

2

2300

1.3

3

2400

2.8

4

2500

1.8

5

2600

1.2

0

1

2

3

4

5

6

7

8

9

DEL

+

Hz

kHz

MHz

GHz

3c. Delete correction point

- Move the cursor to the target using the Arrow key.
- Press F2 (Delete). The frequency and gain are deleted together.

Delete

F 2
- To undo the last deletion, press F4 (Undelete).

Undelete

F 4

Example: point 3 deleted

Pt.	Freq. (MHz)	Gain		Pt.	Freq. (MHz)	Gain
1	2200	2.5	→	1	2200	2.5
2	2300	1.3		2	2300	1.3
3	2400	2.8		3	2500	1.8
4	2500	1.8		4	2600	1.2
5	2600	1.2		5		

#### 4. Save correction set

1. Press F5 (Save Now). The edited data is saved internally.

Save Now **F 5**

2. Press F6 (Return) to go back to the previous menu.

Return **F 6**

#### 5. Activate correction

1. Press F2 (Correction On) to turn On the correction.


Correction On Off **F 2**

2. The amplitude icon appears at the bottom of the display.



#### After correction

Frequency response becomes linear (original), and the gain is compensated by +2 ~ +3dB.

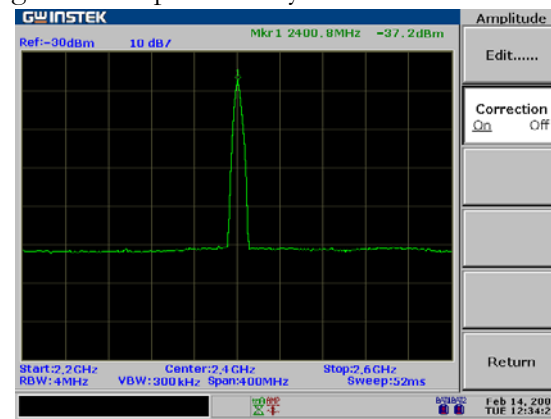

### Delete entire correction set data

#### Panel operation

1. Press the Amplitude key.

Amplitude

2. Press F5 (Corrections).

Corrections.. **F 5**

3. Press F1 (Edit). The display shows the correction sets.

Edit... **F 1**

4. Press F1 (Select) repeatedly to select the correction set.

Select 1 2 3 4 5 **F 1**

5. Press F3 (Delete All).

Delete All.. **F 3**



6. Select and press F1 (No) or F2 (Yes) for confirm. The whole data in the specified correction set is deleted.	No	F 1
	Yes	F 2
7. Press F6 (Return) repeatedly to go back to previous menus.	Return	F 6

### Recall existing correction set


Panel operation	1. Press the Amplitude key.	Amplitude
	2. Press F5 (Corrections).	Corrections.. F 5
	3. Press F1 (Edit). The display shows the correction sets.	Edit... F 1
	4. Press F1 (Select) repeatedly to select the correction set.	Select 1 2 3 4 5 F 1
	5. Press F6 (Return) to go back to the previous menu.	Return F 6
	6. Press F2 (Correction On) to activate the correction.	Correction On Off F 2

### Save/copy/delete/rename correction file


Background	Correction files can be saved, copied, deleted, or renamed using the file utility. Press the File key to access each function.	File
Save/Copy	Press F1 (Copy). For detailed step, see page118.	Copy... F 1
Delete	Press F2 (Delete). For detailed step, see page121.	Delete... F 2
Rename	Press F3 (Rename). For detailed step, see page123.	Rename... F 3

## Use Pre-Amplifier GAP-801 (Optional)

Background	The optional pre-amplifier GAP-801 boosts weak input signals such as in EMI testing to levels that are easy to handle, over the entire frequency range.	
Range	Frequency	9.0kHz ~ 3.0GHz
	Amplitude	11.5dB typical
Connection	<ol style="list-style-type: none"> <li>1. Connect the pre-amplifier GAP-801 between the input terminal and DUT signal output.</li> <li>2. Connect GAP-801 power input to GSP-830 DC 9V output.</li> </ol>	

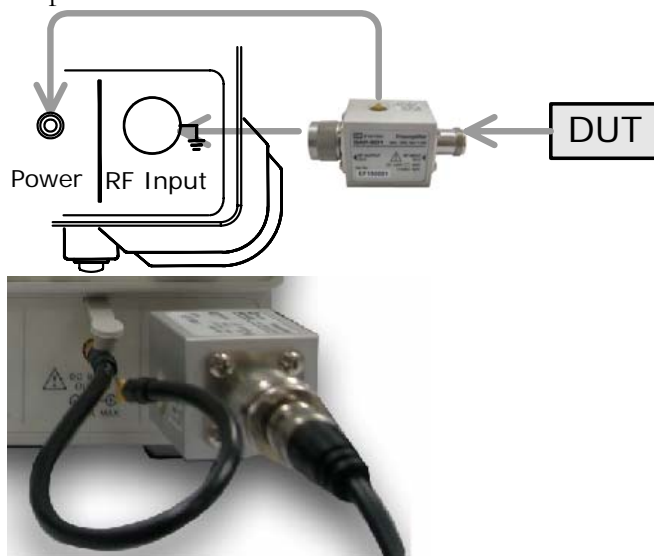







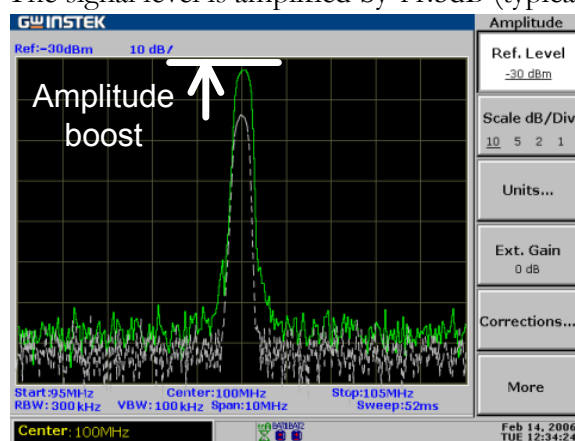3. The signal level is amplified by 11.5dB (typical).











格式化: 標題 2

## Set Input Impedance

### Select input impedance (50Ω/75Ω)

Background	In most cases, the default 50Ω is appropriate. Use 75Ω when specifically required, such as in Cable TV signals.	
Panel operation	1. Press the Amplitude key.	
	2. Press F6 (More).	 
	3. Press F1 (Input Z 50Ω/75Ω) to select the impedance.	 
	4. When 75Ω is selected, the amplitude icon appears at the bottom of the display.	


### Set impedance offset (75Ω only)

Background	Impedance transformation to 75 Ω is also available through external devices such as impedance converter module (GW part No.ADP-101). In these cases an external loss will be induced. The impedance offset can compensate this effect.	
Panel operation	1. Press the Amplitude key.	
	2. Press F6 (More).	 
	3. Make sure 75Ω is selected in F1 (Input Z).	 
	4. Press F2 (Input Z Cal).	 
	5. Enter the offset using the numerical keys.	
Range	−10dB~+10dB, 0.1dB resolution	




格式化: 標題 1

# AUTOSET


**Autoset** function checks the input signal configuration and automatically setup the suitable horizontal and vertical scale. The amplitude floor for limiting the search range, and frequency observation span for limiting the viewing range are customizable according to the application needs.

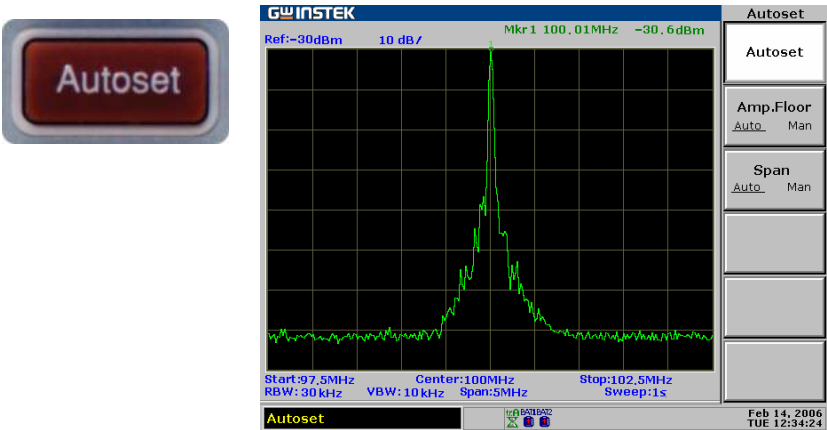


## Run Autoset (search full amplitude range)

Panel operation	1.	Press the Autoset key.	
	2.	Press F1 (Autoset).	 
Search range	Amplitude	dBm	-80 ~ +20dBm
		dBmV	-33.01~+66.99dBmV
		dBuV	+26.99~+126.99dBuV
	Frequency	0kHz ~ 3.0GHz	
	* These ranges are applicable when both Amplitude floor (F2) and Span limit (F3) are set to Auto.		

Example: before Autoset	Start frequency: 0kHz	Stop frequency: 3GHz
	Span: 3GHz	Signal peak: 100MHz
	Center frequency: 1.5GHz	Reference level: -10dBm

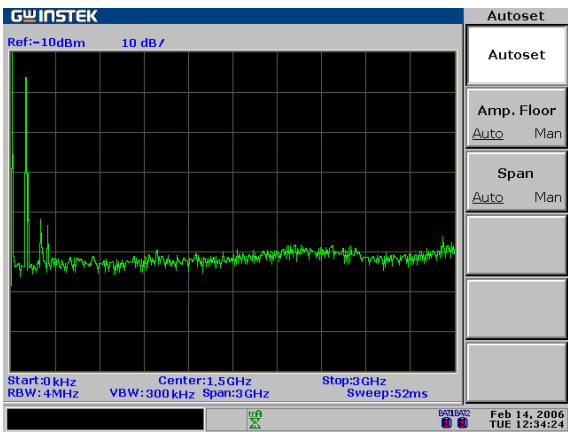

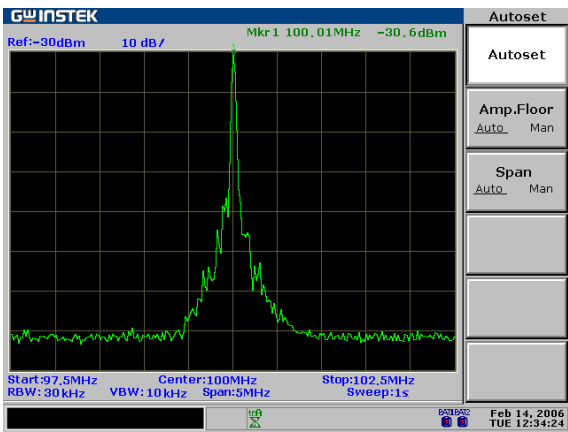


Example: after Autoset	Start frequency: 97.5MHz	Stop frequency: 102.5MHz
	Span: 5MHz	Signal peak: 100MHz
	Center frequency: 100MHz	Reference level: -30dBm






RBW/VBW/Sweep Setting after Autoset	All the three BW related parameters, RBW, VBW, and Sweep, will be reset to Auto mode when using Autoset, regardless of their previous settings.
-------------------------------------	---



Limit vertical search range

Background	You can set the amplitude floor so that the signals lower than the setting will be ignored from Autoset search.	
Panel operation	1. Press the Autoset key.	
	2. Press F2 (Amp. Floor) to switch the range from Auto (whole range) to manual (limited range).	
	3. Enter the amplitude in dB, using the numerical keys. The Command window shows the setting.	
Range	dBm	-80 ~ +20dBm, 0.1dB resolution
	dBmV	-33.01 ~ +66.99dBmV, 0.01dB resolution
	dBuV	+26.99 ~ +126.99dBuV, 0.01dB resolution


Limit horizontal view range

Background	You can change the frequency span limit in the display to get a better view of the Autoset result. By default, the frequency span after Autoset is set at 5MHz (Auto).	
Panel operation	1. Press the Autoset key.	
	2. Press F3 (Span) to switch the range between Auto (5MHz fixed limit) to Manual.	
	3. Enter the frequency using the numerical keys. The Command window shows the setting.	
Range	Zero span, 2kHz ~ 3GHz (Manual) 5MHz fixed (Auto)	

格式化: 標題 1

# MARKER


A **Marker** shows the frequency and amplitude of a waveform point. GSP-830 can activate up to 5 Markers or Marker pairs simultaneously. Marker Table helps editing and viewing multiple Markers in a single display. You can also enable/disable all Markers at once. Delta Marker shows the frequency and amplitude difference between the reference Marker. GSP-830 can automatically move the Marker to various locations including peak signal, center frequency, and start/stop frequency. More Marker operations regarding signal peaks are also available in the **Peak Search** function.

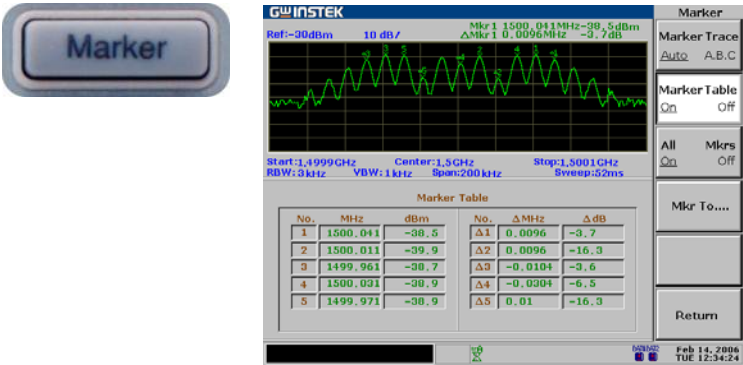

## Activate/de-activate marker(s)

Menu tree

F3 ~ F5 are available only when the Marker is On (activated).

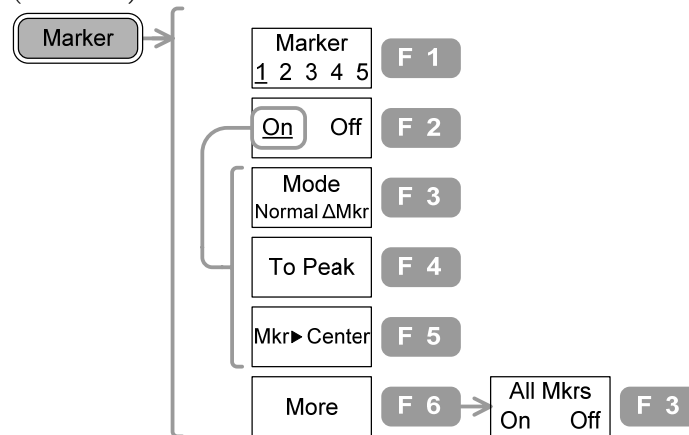

Range	Normal marker	5
	Delta marker	5 pairs
	Amplitude	-120 ~ +20dBm, 0.1dB resolution -73.01~+66.99dBmV, 0.01dB resolution -13.01~+126.99dBuV, 0.01dB resolution
	Frequency	0kHz ~ 3.0GHz


## Activate normal marker(s)

Panel operation	1. Press the Marker key.	
	2. Press F1 (Marker) repeatedly to select the marker ID from 1 to 5.	
	3. Press F2 (On) and turn On the selected marker.	
	4. Make sure Normal is selected in F3. If necessary, press and select Normal.	
	5. Repeat the above steps for the number of markers required.	



Display

The upper right corner of the display shows the active marker.

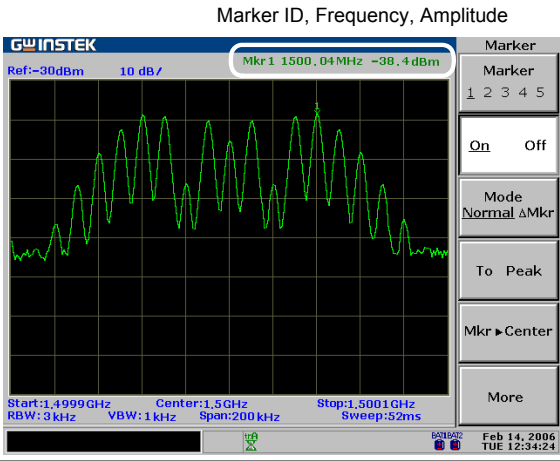

Activate all 5 normal markers at once

- Panel operation
1. Press the Marker key.

Marker
2. Press F6 (More).


More F 6
3. Press F3 (All Mkrs On) to turn On all 5 normal markers.

All Mkrs On Off F 3
4. To view all marker status, press F2 (Marker Table On). The frequency and the amplitude of the markers appear in table list.

Marker Table On Off F 2





Display

The upper right corner of the display shows the active marker status.

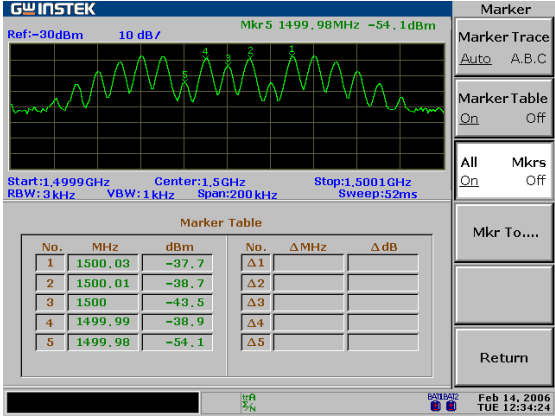


## Activate delta marker(s)

### Panel operation

1. Press the Marker key. 
2. Press F1 (Marker) repeatedly to select the marker ID from 1 to 5. 
3. Press F2 (On) and turn On the selected marker. 
4. Make sure  $\Delta$  (delta) is selected in F3. If necessary, press and select  $\Delta$ Mkr. 
5. Repeat the above steps for the number of markers required.

### Display



The upper right corner of the display shows the active delta marker pair.

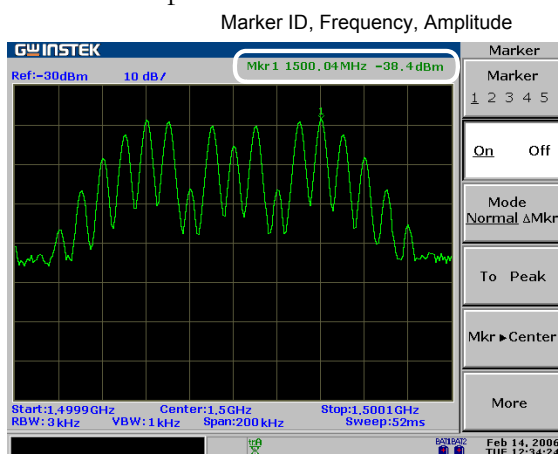










# Move marker(s)

This section assumes at least one marker is already activated (page64). Marker frequency positions can be set manually, or to specific locations using the menu shortcuts.










## Move marker manually

Panel operation	1. Check the active marker at the top right corner of the display.	
	2. Move the marker using the Left/Right key and Scroll knob, or enter the frequency directly using the numerical keys.	



















## Move marker to the highest peak

Method 1	1. Check the active marker at the top right corner of the display.	
	2. Press the Marker key.	
	3. Press F4 (To Peak).	
Method 2	1. Another method (the same effect) is to press the Peak Search key.	
	2. Press F1 (Pk Search).	
Method 3 (marker tracked to the peak)	1. Another method moves marker to the peak and also tracks it. Press the Peak Search key.	
	2. Press F6 (More).	
	3. Press F4 and Turn On the Track.	
	4. The peak tracking icon appears at the bottom of the display.	





## Move marker and the highest peak to the center

Method 1	1. Check the active marker at the top right corner of the display.	
	2. Press the Marker key.	
	3. Press F4 (To Peak). The marker moves to the signal peak.	 
	4. Press F5 (Mkr→Center). The signal peak moves to the center.	 
Method 2	1. Another method (the same effect) is to press the Peak Search key.	
	2. Press F5 (Mkr→Center) to find out the signal peak, then to move it to the center.	 





## Move marker to various locations


Panel operation	1. Check the active marker at the top right corner of the display.	
	2. Press the Marker key.	
	3. Press F6 (More).	 
	4. Press F4 (Mkr to...)	 
	5. Select the destination and press F1 (Center) ~ F5 (Ref Lvl).	 
	<b>Center:</b> center frequency <b>Start:</b> start frequency <b>Stop:</b> stop frequency <b>CF Step:</b> set the marker frequency as the frequency step value <b>Ref Lvl:</b> reference amplitude level	       
	6. Press F6 (Return) to go back to the previous menu.	 

Move marker to a trace

Panel operation	1. Check the active marker at the top right corner of the display.	
	2. Press the Marker key.	
	3. Press F6 (More).	
	4. Press F1 (Marker Trace).	
Range	Auto	The marker moves to the active signal/trace.
	Trace A	The marker moves to Trace A.
	Trace B	The marker moves to Trace B.
	Trace C	The marker moves to Trace C.

Show Markers in Table


Panel operation	1. Check the active marker at the top right corner of the display.	
	2. Press the Marker key.	
	3. Press F6 (More).	
	4. Press F2 (Marker Table On).	
	5. The marker ID, frequency, and amplitude list appears at the lower half of the display, updated in real time.	

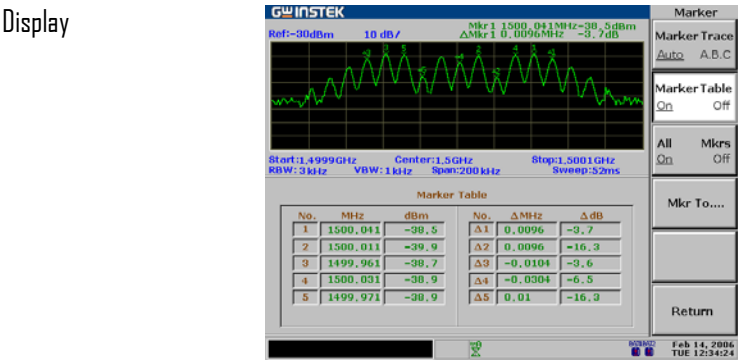

格式化: 標題 1

# PEAK SEARCH

**Peak search** automatically finds out the signal peaks in various conditions, such as next highest peak and minimum peak. Peak Search overlaps its feature with **Marker** function, and it is best to use the two together. All peaks can be viewed at once in the peak table, with amplitude threshold and sorting order configurable.

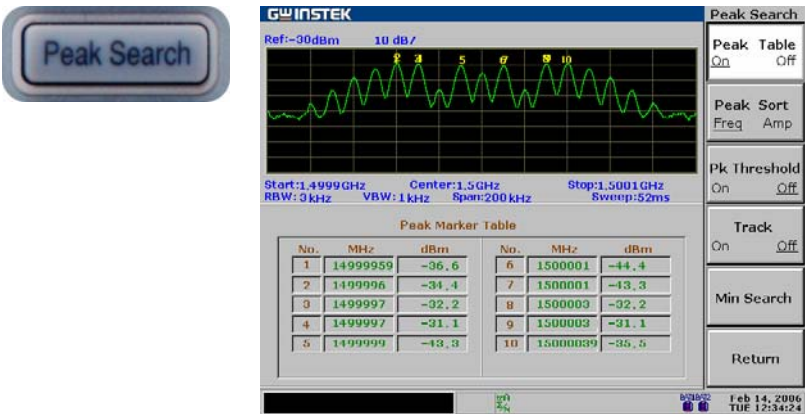


Search signal peaks	Search signal peak.....	71
	Search the next highest peak.....	72
	Search the highest peak and move to the center .....	72
	Search the minimum amplitude .....	73
Show peak table	Activate peak table .....	73
	Set peak threshold.....	74
	Sort peaks .....	74

# Search Signal Peaks

Peak Search puts a marker on the target signal peak. If no marker has been activated, GSP-830 automatically activates marker 1. The peak signal frequency and amplitude appear at the top right corner of the display.

Marker ID, Frequency, Amplitude

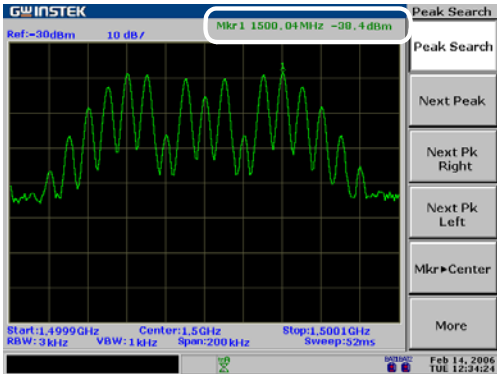








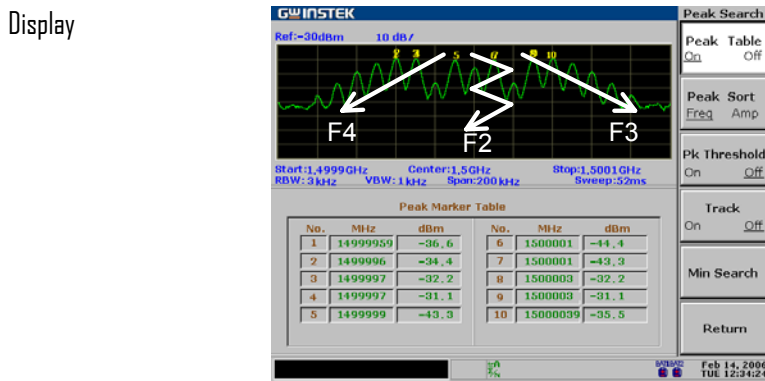
## Search signal peak

Method 1	1. Press the Peak Search key.	<div>Peak Search</div>	
	2. Press F1 (Pk Search).	<div>Pk Search</div>	<div>F 1</div>
Method 2	1. Another method is to use the Marker key. Make sure the marker is already activated (page64).		
	2. Press the Marker key.	<div>Marker</div>	
	3. Press F4 (To Peak).	<div>To Peak</div>	<div>F 4</div>
Method 3 (marker tracked to the peak)	1. Another method continuously tracks the peak signal. Press the Peak Search key.	<div>Peak Search</div>	
	2. Press F6 (More).	<div>More</div>	<div>F 6</div>
	3. Press F4 (Track On).	<div>Track On Off</div>	<div>F 4</div>
	4. The peak tracking icon appears at the bottom of the display.	<div>PTK</div>	









## Search the next highest peak

The marker keeps moving to the next highest peak, in descending order.

Panel operation	1. Press the Peak Search key.	
	2. Press F2 ~ F4 repeatedly. <b>Next Peak:</b> moves the marker to the next highest peak. <b>Next Pk Right:</b> moves the marker to the next highest peak on the right side (higher frequency). <b>Next Pk Left:</b> moves the marker to the next highest peak on the left side (lower frequency).	     



## Search the highest peak and move to the center

Method 1	1. Press the Peak Search key.	
	2. Press F1 (Pk Search).	 
Method 2	1. Another method (the same effect) is to press the Marker key. Make sure the marker is already activated (page64).	
	2. Press the Marker key.	
	3. Press F4 (To Peak).	 
	4. Press F5 (Mkr→Center).	 




Search the minimum amplitude

### Panel operation



1. Press the Peak Search key.



2. Press F6 (More).



3. Press F5 (Min Search). The active marker moves to the deepest valley in the trace.

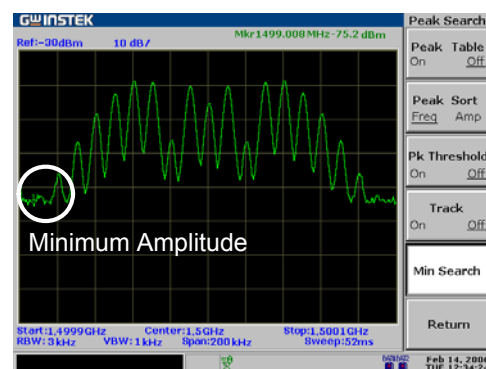

### Show Peak Table


## Activate peak table

## Panel operation



1. Press the Peak Search key.



2. Press F6 (More).



3. Press F1 (Peak Table On).

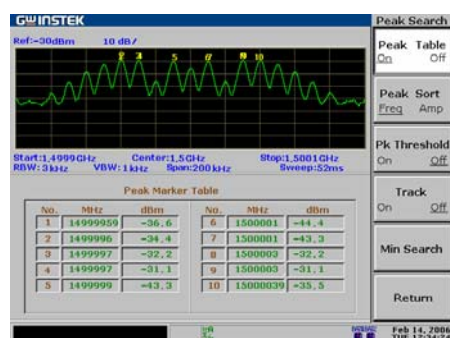










## Range

10 peaks maximum






Set peak threshold

Only the peaks below the threshold amplitude will be listed in the table.


Panel operation	1. Press the Peak Search key.	
	2. Press F6 (More).	 
	3. Press F1 (Peak Table On).	 
	4. Press F3 (Pk Threshold On).	 
	5. A horizontal line appears on the display. GSP-830 searches and lists peaks only below this threshold amplitude.	
	6. Use the Arrow key or the Scroll knob to move the threshold line.	 

Sort peaks

The peaks are sorted in order of ascending frequency / descending amplitude.

Panel operation	1. Press the Peak Search key.	
	2. Press F6 (More).	 
	3. Press F2 (Peak Sort) to switch between frequency and amplitude sorting.	 

Example: amplitude sort


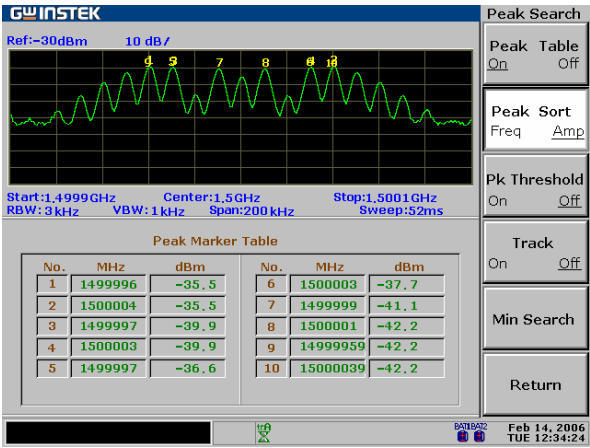


格式化: 標題 1

# T RACE

**Trace** keeps track of waveform variants. Three traces, A, B, and C, are available for accumulating the peak level, freezing the current waveform shape, and averaging the waveform. Trace math operations are available using trace A and B.



Detection modes configure the way GSP-830 samples the input analog signal for digitizing.

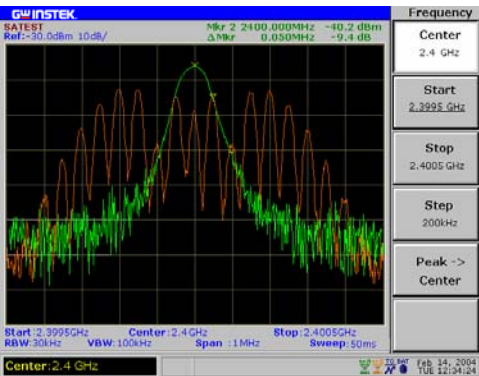




View trace	Select (activate) trace.....	76
	View real-time updated trace (default) .....	76
	View peak-hold trace.....	76
	Freeze trace.....	77
	Hide trace.....	77
	View averaged trace .....	77
Move Trace	Move Marker to Trace .....	78
	Save/copy/delete/rename trace file.....	79
Trace Math	Run Trace Math .....	80
Detection Mode	Select Signal Detection Mode .....	82

# View traced waveform



## Select (activate) trace


Panel operation	1. Press the Trace key.	
	2. Press F1 (Trace) repeatedly to select the trace.	
Range	A (green)	The default trace which is always activated. Together with trace B, runs trace math operation (page80).
	B (amber)	Together with trace A, runs trace math operation (page80).
	C (yellow)	

## View real-time updated trace (default)


Background	The trace is updated at every sweep. Old trace is cleared up and a new trace according to the latest measurement is drawn on the display.	
Panel operation	1. Press the Trace key.	
	2. Press F2 (Clear).	
	3. The clear mode icon appears at the bottom of the display.	

## View peak-hold trace

Background	In peak hold mode, the amplitude of the new trace is compared with the last one at each sweep. Only the higher amplitude replaces old trace points, thus holding the highest (peak) value.	
Panel operation	1. Press the Trace key.	
	2. Press F3 (Peak Hold).	





3. The peak hold mode icon appears at the bottom of the display.
- 

Display

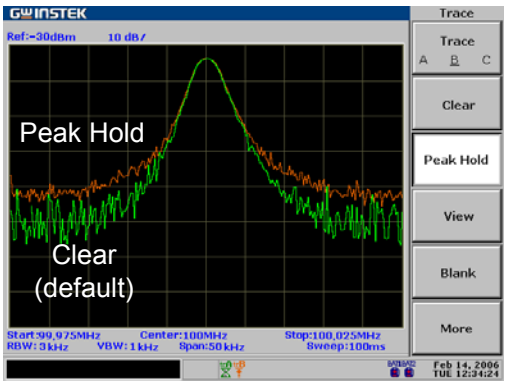






Freeze trace

Panel operation

1. Press the Trace key.
- 
2. Press F4 (View).
- 
3. The view mode (freeze) icon appears at the bottom of the display.
- 




Hide trace









Panel operation

1. Press the Trace key.
- 
2. Press F5 (Blank).
- 
3. The trace disappears from the display. To bring back the trace again, press F2 (Clear).
- 

View averaged trace


Panel operation (Method1)

1. Press the Trace key.
- 
2. Press F6 (More).
- 








	3. Press F1 (AVG On) to turn On the average mode.		
	4. The average mode icon appears at the bottom of the display.		
	5. Enter the average number using the numerical keys.		
Method2	1. Press the BW key.		
	2. Press F4 (AVG On) to turn On averaging.		
	3. Enter the average time using the numerical keys.		
Range	1 ~ 100		

Example: after average

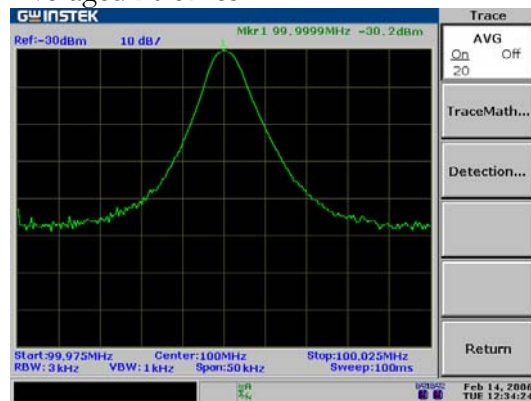Averaged 20 times




## Move Marker to Trace

Panel operation	1. Check the active marker at the top right corner of the display.		
	2. Press the Marker key.		
	3. Press F6 (More).		
	4. Press F1 (Marker Trace).		
Range	Auto	The marker moves to the active signal or trace.	

Trace A	The marker moves to Trace A.
Trace B	The marker moves to Trace B.
Trace C	The marker moves to Trace C.

Display

Marker on Trace C

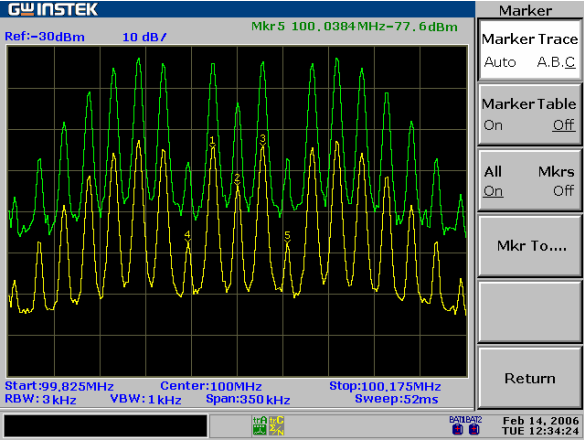

Save/copy/delete/rename trace file


















Background	Trace files can be saved, copied, deleted, or renamed using the file utility. Press the File key to access each function.	<div>File</div>
Save/Copy	Press F1 (Copy). For detailed step, see page118.	<div>Copy...F 1</div>
Delete	Press F2 (Delete). For detailed step, see page121.	<div>Delete...F 2</div>
Rename	Press F3 (Rename). For detailed step, see page123.	<div>Rename...F 3</div>

## Run Trace Math


### Background

You can run various mathematical operations between TraceA and TraceB. Both traces have to be activated (page76) in advance. After the math operation, the traces mode changes into View (page77).

### Panel operation



1. Press the Trace key. 
2. Press F6 (More).  
3. Press F2 (Trace Math).  
4. Select and press the type of math operation from F1 ~ F5.  
 $A \leftrightarrow B$ : swaps trace A and B.    
 $A+B \rightarrow A$ : Adds trace A and B.    
 $A-B \rightarrow A$ : Subtracts trace B from trace A.    
 $A+const \rightarrow A$ : Adds a constant value to trace A.    
 $A-const \rightarrow A$ : Subtracts a constant value from trace A.  
5. When  $A+const$  /  $A-const$  are selected, enter the constant value using the numerical keys. Range:  $-40 \sim +40\text{dB}$  
6. The trace math icon appears at the bottom of the display. 

### Example: $A \leftrightarrow B$


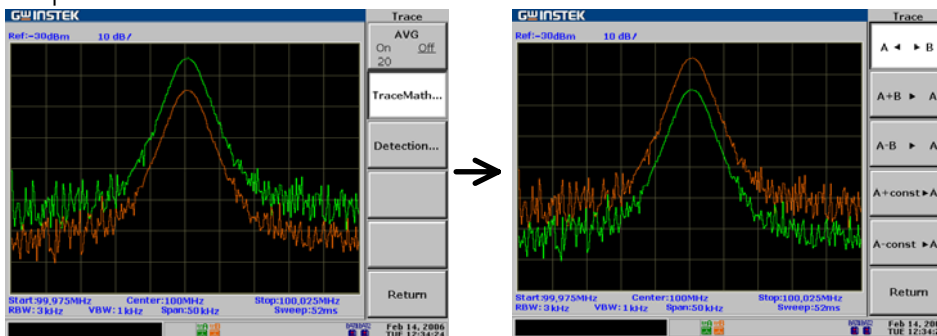






Example:  $A+B \rightarrow A$

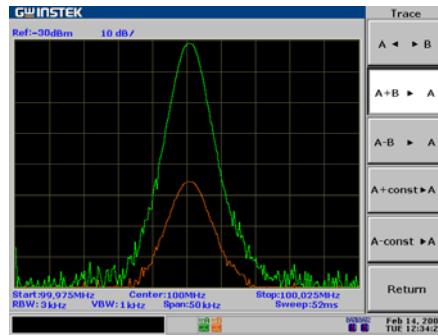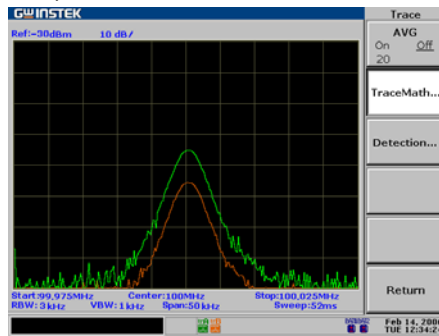



Example:  $A-B \rightarrow A$

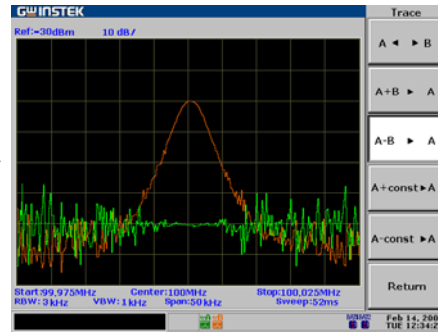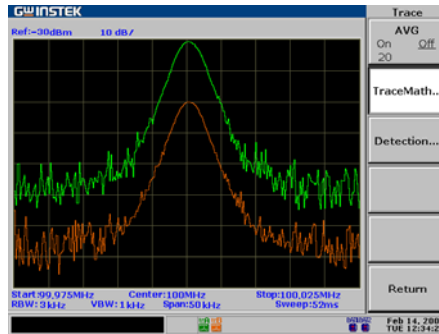







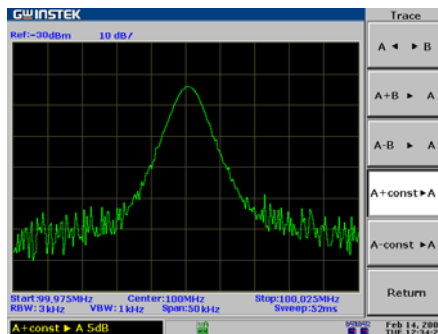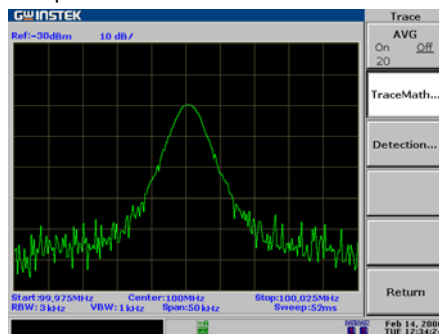










Example:  $A+\text{constant} \rightarrow A$  (5 dB)

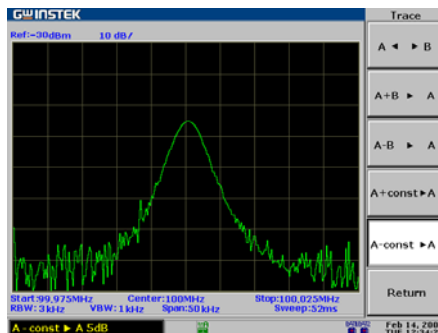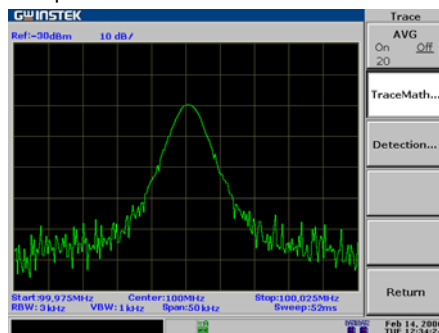

Example:  $A-\text{constant} \rightarrow A$  (5 dB)




## Select Signal Detection Mode

Background	In order to show the incoming signal on the display, GSP-830 first converts the input signal to a video signal, digitizes it, then use a detector to pick up the samples to be displayed. By configuring the detection mode, certain signals can be viewed more clearly/sharply.	
Panel operation	1. Press the 'Trace' key.	
	2. Press F6 (More).	 
	3. Press F3 (Detection).	 
	4. Select the signal detection type from F1 ~ F5 and press it. See below for description of each type.	 
		 
		 
		 
		 
Parameter	5. Press F6 (Return) to go back to the previous menu.	 
	Normal	The default mode. When the signal level is constantly increasing or decreasing detects the positive peaks. Otherwise, detecting mode switches between positive peak and negative peaks. Useful for picking up burst phenomenon while avoiding too much noise.
	Sample	Detects signals randomly. Useful when detecting noise-like signals, but tend to miss burst phenomenon.
	Peak+ (positive peak)	Detects positive peak signals. Useful for detecting sinusoid signal, but tend to pick up more noise than other modes.


AVG (average)	Available when the optional EMI filter is installed. Detects the average power level of the samples, using low pass filter. Useful for reducing the noise level. For EMI filter details, see page149.
QPeak (quasi-peak)	Available when the optional EMI filter is is installed. Detects the quasi-peak power level of the samples. Useful for viewing in zero span without missing signal variations. For EMI filter details, see page149.

Example

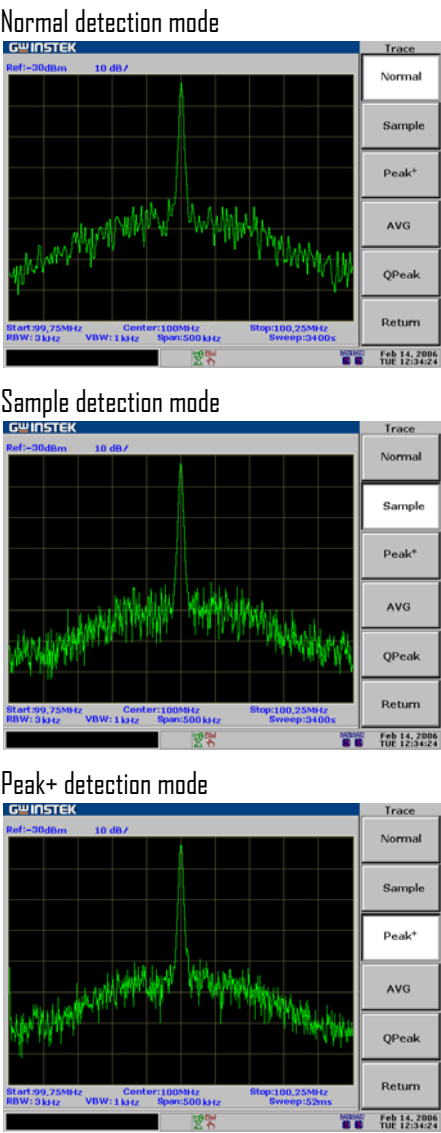

# P OWER MEASUREMENT

**Power Measurement** function includes four types of frequently used complex measurement items: ACPR, OCBW, N dB, and Phase Jitter. Each item is configurable and updated in real-time.

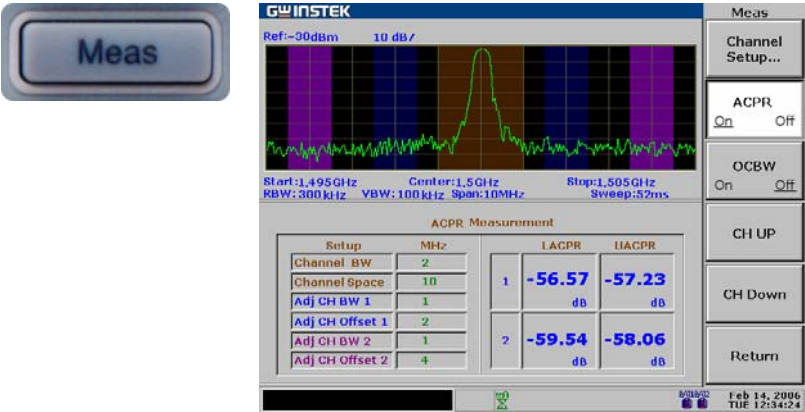


ACPR	Overview .....	85
	ACPR measurement step .....	86
OCBW	Overview .....	88
	OCBW measurement step.....	88
N dB	N dB Measurement .....	90
Phase Jitter	Phase Jitter Measurement .....	91

# ACPR Measurement

## Overview

Background

ACPR (Adjacent Channel Power Ratio), or ACLR (Adjacent Channel Leakage Ratio) in other term, refers to the amount of leakage power coming from the main radio channel which affects adjacent channels as signal distortion.

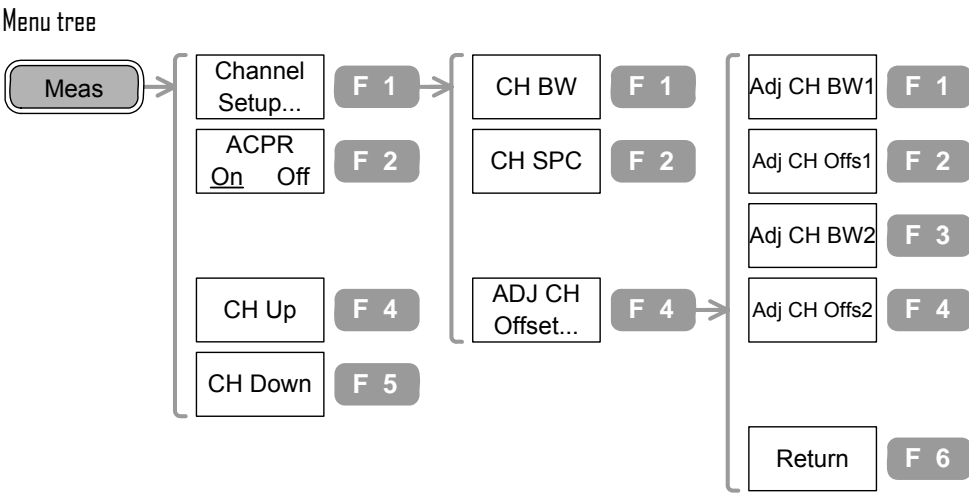


Parameter	Channel bandwidth	The frequency bandwidth that the target channel occupies. 1kHz ~ 3.0GHz
	Channel space	The frequency distance between each main channel. 1kHz ~ 3.0GHz
	Adjacent channel bandwidth 1 & 2	The frequency bandwidth that the adjacent channels 1 & 2 occupy. 1kHz ~ 3.0GHz
	Adjacent channel offset 1 & 2	The frequency distance between the adjacent channel 1 & 2 and the main channel. 1kHz ~ 3.0GHz


## ACPR measurement step

### I. Activate ACPR


1. Press the Measurement key.



2. Press F2 (ACPR On).




3. The display switches to ACPR mode, showing and updating ACPR result on the lower half.

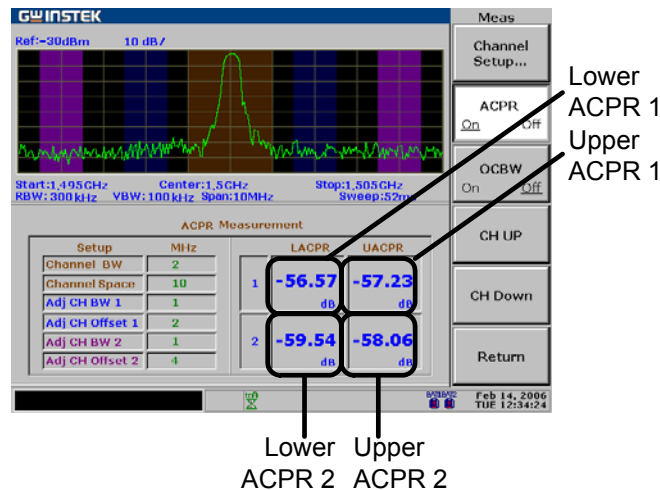


### 2. Set channel BW

1. Press F1 (Channel Setup).



2. Press F1 (CH BW).



3. Enter the channel BW using the numerical keys, in MHz.  
Range: 1kHz ~ 3.0GHz



4. The value is updated at the channel BW column.



### 3. Set channel space

1. Press F2 (Channel SPC).







2. Enter the channel space using the numerical keys, in MHz.  
Range: 1kHz ~ 3.0GHz



3. The value is updated at the channel space column.




4. Set adjacent channel1 bandwidth	1. Press F4 (ADJ CH Offset).	ADJ CH Offset...	F 4
	2. Press F1 (Adj CH BW1).	Adj CH BW1	F 1
	3. Enter the adjacent channel 1 bandwidth using the numerical keys. Range: 1kHz ~ 3.0GHz		
	4. The value is updated at the Adj CH BW1 column.	Adj CH BW 1	1
5. Set adjacent channel1 offset	1. Press F2 (Adj CH Offs1).	Adj CH Offs1	F 2
	2. Enter the adjacent channel 1 offset using the numerical keys. Range: 1kHz ~ 3.0GHz		
	3. The value is updated at the Adj CH Offset1 column.	Adj CH Offset 1	2
6. Set adjacent channel2 bandwidth	1. Press F3 (Adj CH BW2).	Adj CH BW2	F 3
	2. Enter the adjacent channel 2 bandwidth using the numerical keys. Range: 1kHz ~ 3.0GHz		
	3. The value is updated at the Adj CH BW2 column.	Adj CH BW 2	1
7. Set adjacent channel2 offset	1. Press F4 (Adj CH Offs2).	Adj CH Offs2	F 4
	2. Enter the adjacent channel 2 offset using the numerical keys. Range: 1kHz ~ 3.0GHz		
	3. The value is updated at the Adj CH Offset2 column.	Adj CH Offset 2	4
8. Move channel up/down	1. Press F6 (Return) twice.	Return	F 6
		x2	
	2. Press F4 (CH Up) or F5 (CH Down) to switch the measurement to the next channel.	CH Up	F 4
		CH Down	F 5

# OCBW Measurement

## Overview

**Background** OCBW (OCcupied BandWidth) refers to the bandwidth of the channel that consumes (occupies) the specified amount of power.

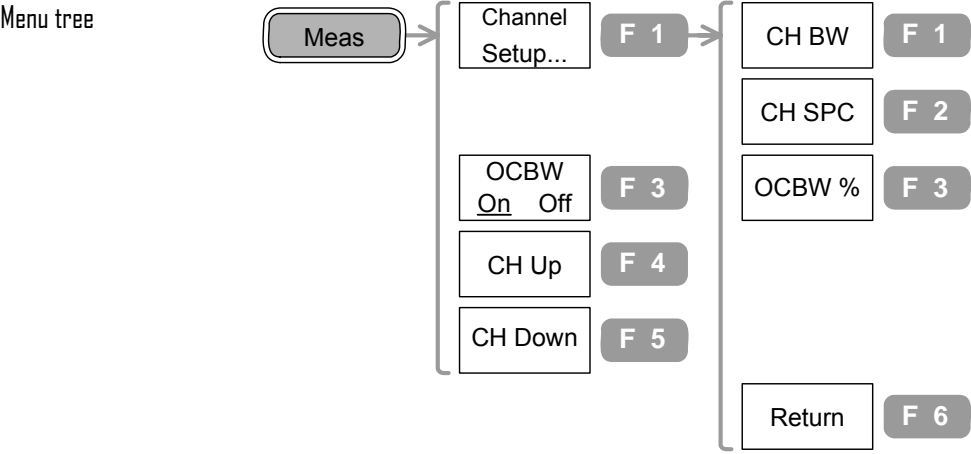

Parameter	Channel bandwidth	The frequency bandwidth that the target channel occupies. 1kHz ~ 3.0GHz, 1kHz resolution
	Channel space	The frequency distance between each main channel. 1kHz ~ 3.0GHz, 1kHz resolution
	OCBW %	The ratio of occupied bandwidth as the amount of power consumed. 0.0% ~ 100.0%, 0.1% resolution

## OCBW measurement step

- I. Activate OCBW

1. Press the Measurement key.


Meas

2. Press F3 (OCBW On).

OCBW On Off F 3

3. The display switches to OCBW mode, showing and updating OCBW result on the lower half.



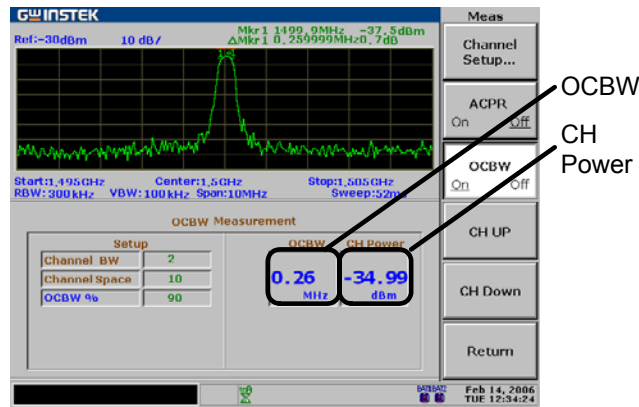

2. Set channel BW	1. Press F1 (Channel Setup).	Channel Setup...	F 1
	2. Press F1 (CH BW).	CH BW	F 1
	3. Enter the channel BW using the numerical keys, in MHz. Range: 1kHz ~ 3.0GHz		
	4. BW column updates the value.		
3. Set channel space	1. Press F2 (Channel SPC).	CH SPC	F 2
	2. Enter the channel space using the numerical keys, in MHz. Range: 1kHz ~ 3.0GHz		
	3. Space column updates the value.		
4. Set OCBW %	1. Press F3 (OCBW %).	OCBW %	F 3
	2. Enter the OCBW % using the numerical keys and Enter key. Range: 0.0% ~ 100%		
	3. OCBW % column updates the value.		
5. Move channel up/down	1. Press F6 (Return) twice.	Return	F 6
	2. Press F4 (CH Up) or F5 (CH Down) to switch the measurement to the next channel.	CH Up CH Down	F 4 F 5

# N dB Measurement

Background N dB refers to the frequency bandwidth of a channel that covers the specified amplitude.

Parameter N dB 0.1dB ~ 80.0dB, 0.1dB resolution

- I. Activate N dB
1. Press the Measurement key.


Meas
2. Press F6 (More).

More

F 6
3. Press F1 (N dB BW On).

N dB BW  
On Off

F 1
4. The display switches to N dB mode, showing and updating N dB result on the lower half.

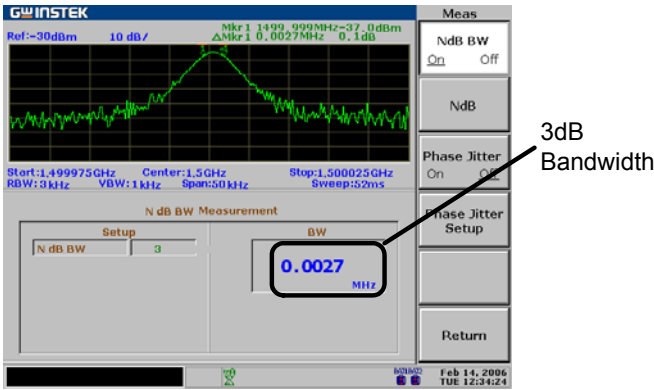

2. Set amplitude
1. Press F2 (NdB) to set the amplitude which the BW covers.

N dB

F 2
2. Enter the amplitude using the numerical keys.

Range: 0.1dB ~ 70.0dB

# Phase Jitter Measurement

Background	Phase Jitter refers to the amount of phase fluctuation that leads to shortening or lengthening the Center frequency.	
Parameter	Start offset	Beginning frequency offset in reference to the center frequency. 0.0MHz ~ 1/2 of Span, 0.1MHz resolution
	Stop offset	End frequency offset in reference to the center frequency. 0.0MHz ~ 1/2 of Span, 0.1MHz resolution

1. Activate Phase Jitter
1. Press the Measurement key.


Meas
2. Press F6 (More).

More

F 6
3. Press F3 (Phase Jitter On).

Phase Jitter On Off

F 3
4. The display switches to Phase jitter mode, showing and updating Phase jitter result on the lower half.

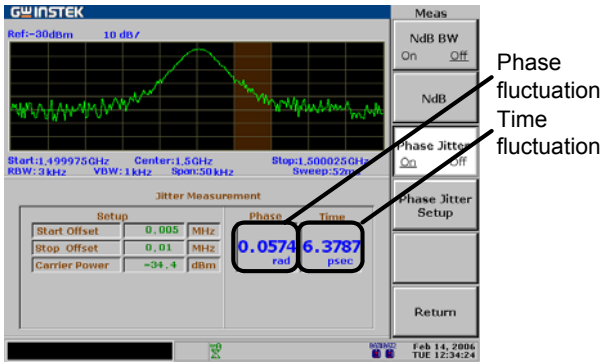

2. Set start/stop offset
1. Press F4 (Phase Jitter Setup).

Phase Jitter Setup

F 4
2. Press F1 (Start Offset) and F2 (Stop Offset) to set the amount of beginning/end offset.

Start Offset

F 1

Stop Offset


F 2
3. Enter the offset using the numerical keys.

Range: 0.0MHz ~ 1/2 of Span

0 1 2 3 4 5 6 7 8 9

# LIMIT LINE

**Limit Line** sets the upper and lower amplitude limit over the entire frequency range. The limit lines can be used to detect whether the input signal level is above, below, or within the target amplitude. The result, pass or fail, is shown at the display bottom in real-time.

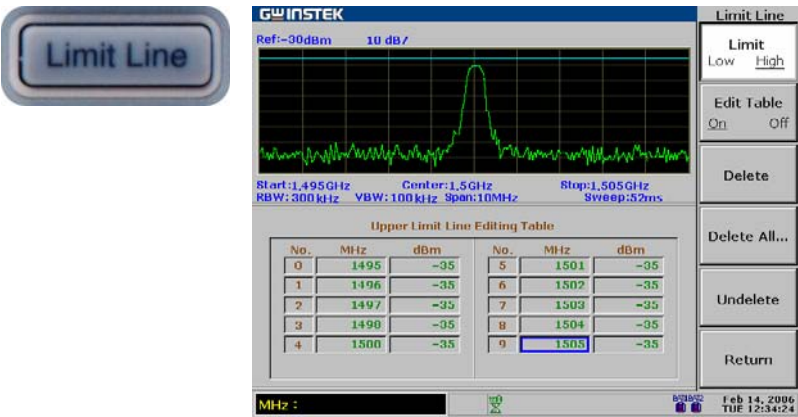


Edit	Edit Limit Line .....	93
Pass/Fail test	Run Pass/Fail test .....	96
Limit Line File	Save/copy/delete/rename limit line file.....	97

## Edit Limit Line


Parameters	Editing point	Maximum 10 points for each High and Low limit line.
	Frequency	9kHz ~ 3.0GHz per editing point.
	Amplitude	Per editing point: -130 ~ +20dBm -83.01dBmV ~ +66.99dBmV -23.01dBuV ~ +126.99dBuV

### 1. Activate Limit Line

1. Press the Limit Line key.
2. Press F1 (H Limit On) and/or F2 (L Limit On) to activate the upper/lower limit line.





3. The limit line appears on the display.
- Blue: — H limit line
- Yellow: — L limit line

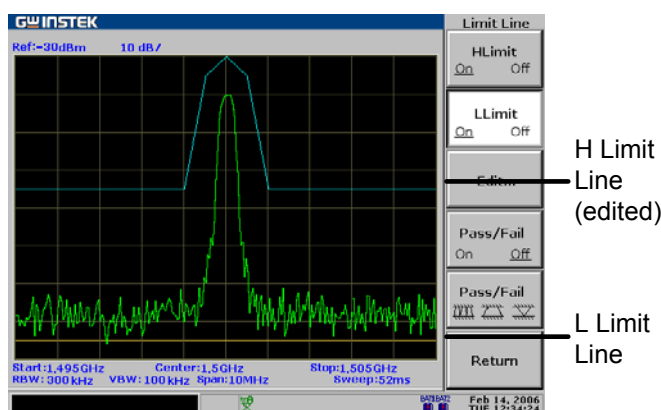

2. Activate limit line editing 1. Press F3 (Edit).

2. Press F1 (Limit) to select the limit line to be edited.
3. Press F2 (Edit Table On). The editing table appears on the bottom half of the display.



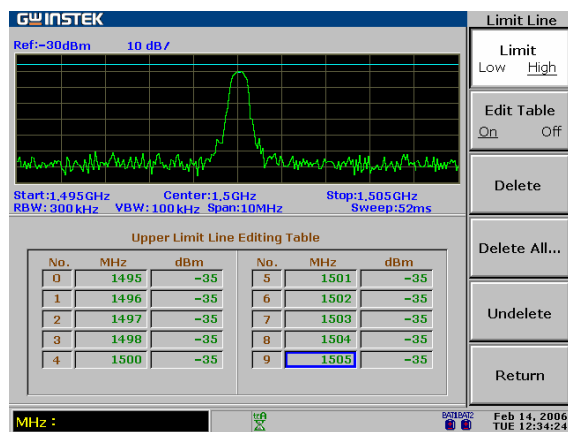

### 3a. Add a limit line point

1. Make sure that the cursor is pointing to the first empty frequency point. Use the Up/Down key to move the cursor, if necessary.  
10 points are available for upper and lower limit line each.

No.	MHz	dBm
1		
2		
3		
4		
5		



2. If necessary, move the cursor to different frequency points using the Arrow key.



3. Enter the frequency in MHz using the numerical keys.  
9.0kHz ~ 3.0GHz.



4. The cursor automatically moves to the Gain side. Enter the gain in dB using the numerical keys.  
Range: -130dB ~ +20dBm

No.	MHz	dBm
1	98	
2		
3		
4		
5		

5. Continue the above steps for the points needed.

### 3b. Delete a limit line point

1. Move the cursor to the deletion point using the Arrow key.
2. Press F3 (Delete) to delete the point (frequency and amplitude together).



No.	MHz	dBm
1	98	-40
2	100	-30
3	102	-40
4		
5		










No.	MHz	dBm
1	98	-40
2	102	-40
3		
4		
5		




## Run Pass/Fail test

This section assumes the limit line is already defined.

Pass/Fail condition		Checks whether all the waveform amplitude stays between the high limit and low limit lines.
		Checks whether the peak amplitude of the waveform stays between the high and low limit lines.
		Checks whether the minimum amplitude of the waveform stays between the high and low limit lines.

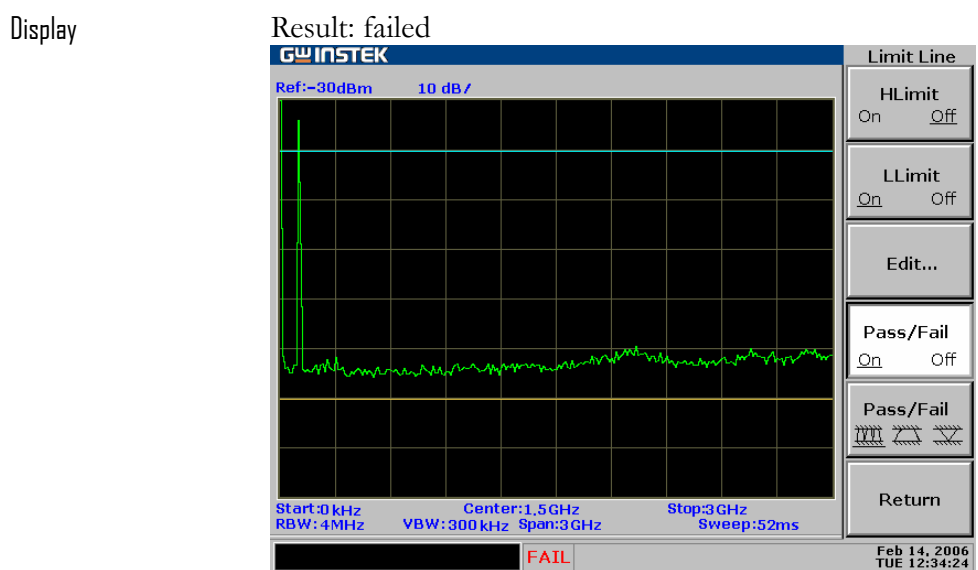






1. Select condition	1. Press the Limit Line key.	
	2. Press F5 (Pass/Fail) repeatedly to select the condition.	
2. Run Pass/Fail test	1. Press F4 (Pass/Fail On) to activate the test.	
	2. The test result appears at the bottom of the display.	



Note	If the high or low limit line is not defined, Pass/Fail test uses the highest or lowest display level as limit line.
------	--




Save/copy/delete/rename limit line file

Background	Limit line files can be saved, copied, deleted, or renamed using the file utility. Press the File key to access each function.	
Save/Copy	Press F1 (Copy). For detailed step, see page118.	 
Delete	Press F2 (Delete). For detailed step, see page121.	 
Rename	Press F3 (Rename). For detailed step, see page123.	 





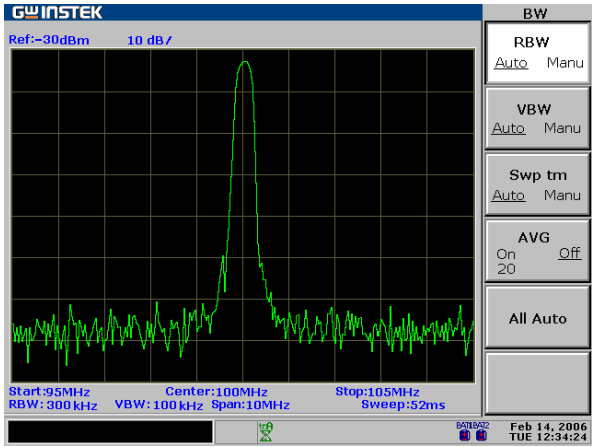


# BANDWIDTH

**BW (BandWidth)** feature configures how narrow GSP-830 can sort out different signal peaks (resolution), and how fast the display can be updated (sweep time). Averaging the waveform is also available for smoothing noise level. The resolution and the sweep time (+averaging) are in a trade-off relationship, so configuration should be done with care.



RBW/VBW	Select RBW (Resolution BandWidth) .....	99
	Select VBW (Video BandWidth) .....	101
	RBW/VBW Auto Mode Contents.....	102
Sweep Time	Set Sweep time.....	104
Average	Average Waveform .....	104
Reset	Reset RBW/VBW/SweepTime to Auto .....	105

# Select RBW (Resolution BandWidth)

Background	RBW (Resolution Bandwidth) defines the width of the IF (intermediate frequency) filter that is used to separate signal peaks from one another. The narrower the RBW, the greater the capability to separate signals at close frequencies. But it also makes the sweep time longer under specific frequency span; the display is updated less frequently. See page102 for the reference to select the suitable RBW.	
Panel operation	1. Press the BW key.	
	2. Press F1 (RBW) to select Auto or Manual.	 
	3. When Manu (manual) is selected, use the Arrow key or Scroll knob to change it.	 
	4. The selected RBW appears in the command window.	
Mode	Auto	RBW is automatically set. See page102 for the setting.
	Manual 	RBW is manually selected. The BW icon appears at the bottom of the display.
Range	See page102 for RBW reference setting according to the frequency span.	
	RBW	Recommended span
	Standard/ Optional	
	300Hz	Span<30kHz
		Optional (300Hz RBW)
	3kHz	Span<300kHz
		Standard
	9kHz	300kHz≤Span<600kHz
		Optional (EMI Filter - page149)
	10kHz	300kHz≤Span<1MHz
		Optional (10k/100kHz RBW)
	30kHz	300kHz≤Span<6MHz
		Standard

100kHz	6MHz≤Span<20MHz	Optional (10k/100kHz RBW)
120kHz	6MHz≤Span<19MHz	Optional (EMI Filter – page149)
300kHz	6MHz≤Span<60MHz	Standard
4MHz	60MHz≤Span	Standard

Check RBW installation  
status

1. Press the System key.


System
2. Press F6 (More).

More...

F 6
3. Press F4 (System Config On) to turn On the system configuration window.

System Config  
On Off

F 4

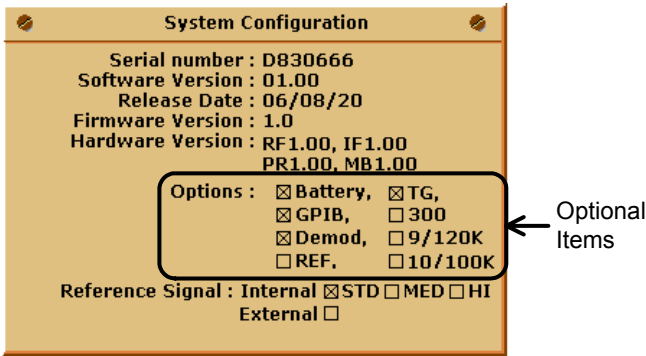

4. Check the optional items corner and see the RBW installation status (checkmark – installed, blank – not installed)

Installed

☒ 300

☒ 9/120K

☒ 10/100K

Not installed

☐ 300

☐ 9/120K

☐ 10/100K
5. Press F4 (System Config Off) to close the system configuration window.






System Config  
On Off

F 4

Note

9k/120kHz RBW (EMI Filter) and 10k/100kHz RBW are exclusive; cannot be installed together. For a new RBW option install, contact service personnel.

# Select VBW (Video BandWidth)

Background	VBW (Video Bandwidth) defines the smoothness of the trace on the display. Combined with RBW, Video BandWidth defines the ability to sort out target signal from surrounding noise or adjacent peaks. See page102 for reference to select the suitable VBW.	
Panel operation	1. Press the BW key.	
	2. Press F2 (VBW) to select Auto or Manual.	
	3. When Manu (manual) is selected, use the Arrow key or Scroll knob to change it.	
	4. The selected VBW appears in the command window.	
Mode	Auto	VBW is automatically set. See page102 for setting.
	Manual 	VBW is manually set. The VBW icon appears at the bottom of the display.
Range	10Hz ~ 1MHz in 1-3 steps  VBW is automatically selected according to the RBW in Auto mode. See page102 for the setting list. Use this for the reference when manually selecting the VBW.	
Note	• GSP-830 automatically changes the VBW according to RBW selection.	

# RBW/VBW Auto Mode Contents

- Background
- The following applies when selecting Auto for RBW and VBW setting. Use them as a reference when manually selecting the RBW and VBW.
  - The RBW/VBW range differs according to system configuration, especially the optional item installation.

Check the RBW installation status

1. Press the System key.

System

2. Press F6 (More).

More... F 6

3. Press F4 (System Config On) to turn On the system configuration window.

System Config On Off F 4

System Configuration

Serial number : D830666  
Software Version : 01.00  
Release Date : 06/08/20  
Firmware Version : 1.0  
Hardware Version : RF1.00, IF1.00  
PR1.00, MB1.00

Options : ☒ Battery, ☒ TG,  
☒ GPIB, ☐ 300  
☒ Demod, ☐ 9/120K  
☐ REF, ☐ 10/100K


Reference Signal : Internal ☒ STD ☐ MED ☐ HI  
External ☐

Optional Items

4. Press F4 (System Config Off) to close the system configuration window.





System Config On Off F 4

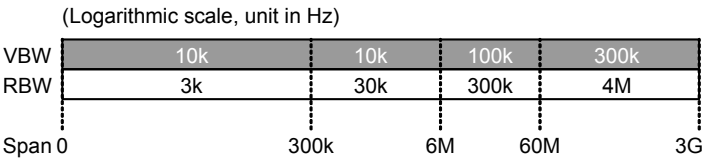Standard configuration	Optional item	Install	Configuration
	EMI Filter(9k/120k RBW)	No	<input type="checkbox"/> 9/120K
	300Hz RBW	No	<input type="checkbox"/> 300
	10k/100kHz RBW	No	<input type="checkbox"/> 10/100K






Standard + 9k/120kHz RBW configuration	Optional item	Install	Configuration
	EMI Filter (9k/120k RBW)	Yes	<input checked="" type="checkbox"/> 9/120K
	300Hz RBW	No	<input type="checkbox"/> 300
	10kHz/100kHz RBW	No	<input type="checkbox"/> 10/100K
(Logarithmic scale, unit in Hz)			
<div> <div>VBW</div> <div>RBW</div> <div>Span 0</div> <div>300k</div> <div>600k</div> <div>6M</div> <div>19M</div> <div>60M</div> <div>3G</div> </div>			
Standard + 300/9k/120kHz RBW configuration	Optional item	Install	Configuration
	EMI Filter (9k/120k RBW)	Yes	<input checked="" type="checkbox"/> 9/120K
	300Hz RBW	Yes	<input checked="" type="checkbox"/> 300
	10kHz/100kHz RBW	No	<input type="checkbox"/> 10/100K
(Logarithmic scale, unit in Hz)			
<div> <div>VBW</div> <div>RBW</div> <div>Span 0</div> <div>30k</div> <div>300k</div> <div>600k</div> <div>6M</div> <div>19M</div> <div>60M</div> <div>3G</div> </div>			
Standard + 10k/100kHz RBW configuration	Optional item	Install	Configuration
	EMI Filter (9k/120k RBW)	No	<input type="checkbox"/> 9/120K
	300Hz RBW	No	<input type="checkbox"/> 300
	10kHz/100kHz RBW	Yes	<input checked="" type="checkbox"/> 10/100K
(Logarithmic scale, unit in Hz)			
<div> <div>VBW</div> <div>RBW</div> <div>Span 0</div> <div>300k</div> <div>1M</div> <div>6M</div> <div>20M</div> <div>60M</div> <div>3G</div> </div>			
Standard + 300/10k/100kHz RBW configuration	Optional item	Install	Configuration
	EMI Filter (9k/120k RBW)	No	<input type="checkbox"/> 9/120K
	300Hz RBW	Yes	<input checked="" type="checkbox"/> 300
	10kHz/100kHz RBW	Yes	<input checked="" type="checkbox"/> 10/100K
(Logarithmic scale, unit in Hz)			
<div> <div>VBW</div> <div>RBW</div> <div>Span 0</div> <div>30k</div> <div>300k</div> <div>1M</div> <div>6M</div> <div>20M</div> <div>60M</div> <div>3G</div> </div>			









## Set Sweep time

Background	Sweep time defines the display update rate. Note that the sweep time and RBW/VBW are in trade-off. Faster sweep time updates display more frequently but makes RBW and VBW wider, reducing the capability to separate signals at close frequencies.	
Panel operation	1. Press the BW key.	
	2. Press F3 (Swp tm) to switch between Auto and Manual setting.	 
	 In Manual mode, the Manual Sweep Time icon appears.	
Mode	Auto	Sweep time is automatically set.
	Manual	Sweep time is manually set.
Range	50ms ~ 12.8s, 1us resolution	
Note	When in Auto mode, GSP830 is optimized for fast sweep time. For narrower RBW settings, like 300 Hz and 3 KHz, this optimization will cause the phase noise slightly higher. To reduce the phase noise level, please slow down the sweep time using manual setting.	





## Average Waveform

Background	GSP-830 averages the waveform for a configured number, then shows on the display. This feature smoothes the noise level to a great extent, but slows down the display update rate.	
Panel operation (Method)	1. Press the BW key.	
	2. Press F4 (AVG On) to turn On averaging.	 




	3.	Enter the average time using the numerical keys.	
Panel operation (Method2)	1.	Press the Trace key.	
	2.	Press F6 (More).	 
	3.	Press F1 (AVG On) to turn On the average mode.	 
	4.	The average mode icon appears at the bottom of the display.	
	5.	Enter the average number using the numerical keys.	
Parameter	1 ~ 200	Only available when Average is On.	

Reset RBW/VBW/SweepTime to Auto

Panel operation	1.	Press the BW key.	
	2.	Press F5 (All Auto). RBW, VBW, and Sweep time setting all changes to Auto.	 
RBW/VBW/Sweep Setting after Autoset	 All the three BW related parameters, RBW, VBW, and Sweep, will be reset to AUTO mode when using Autoset, regardless of their previous settings.		

# T RIGGER

**Trigger** function sets the signal conditions upon which GSP-830 triggers capturing waveforms, including frequency, amplitude, and delay. External signal can be used in case a special condition is required.

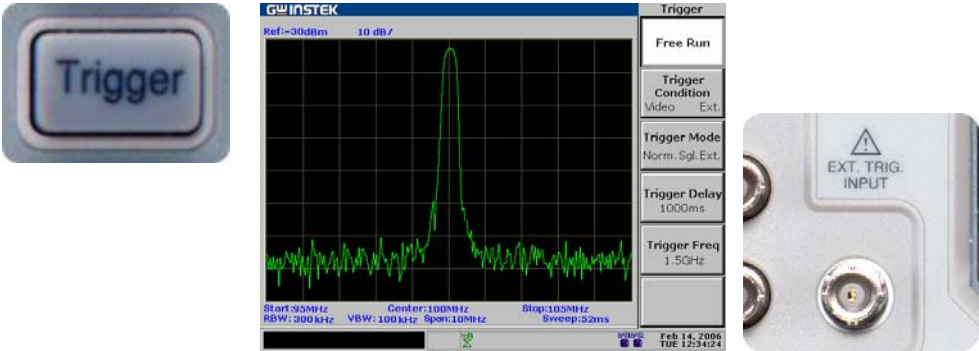




Free Run	Free Run (Default).....	107
Video Trigger	Activate video trigger.....	107
External Trigger	Activate external trigger.....	108
Trigger Mode	Select trigger mode.....	108
Trigger Delay	Set trigger delay.....	109

### Free Run (Default)













In free run, GSP-830 captures all incoming signals (no triggering condition).

Panel operation

1. Press the Trigger key. 
2. Press F1 (Free Run).  

## Activate video trigger





Panel operation

1. Press the Trigger key. 
2. Press F2 (Trigger Condition). Select Video.  
3. The video trigger icon appears at the bottom of the display. 
4. Enter the trigger level (amplitude) using the numerical keys. The value appears in the command window.     
 Video: -20dBm
5. Press F5 (Trigger Freq) to set the frequency at which GSP-830 checks the trigger condition.  
6. Enter the trigger frequency using the numerical keys.  
7. To de-activate triggering, press F1 (Free Run).  




Trigger level range	dBm	-130 ~ +20dBm
	dBmV	-83.01 ~ +66.99dBmV
	dBuV	-23.01 ~ +126.99dBuV

Trigger frequency range 0 ~ 3.0GHz




## Activate external trigger

Panel operation	1. Press the Trigger key.	
	2. Press F2 (Trigger Condition). Select Ext.	
	3. The Ext. trigger icon appears at the bottom of the display.	
	4. Connect the external trigger signal to the rear panel terminal. The positive edge between 0V and 5V triggers GSP-830.	
Input level range	0 ~ 5V, positive edge trigger	

## Select trigger mode


Panel operation	1. Press the Trigger key.	
	2. Press F3 (Trigger Mode) repeatedly to select the trigger modes.	
	3. When Sgl (single) or Cont. (continuous) is selected, you can use F6 (Run Now) to manually start the triggering.	
Modes	Normal	GSP-830 captures signal every time the triggering condition occurs.
	Single	GSP-830 captures signal when the first triggering condition occurs, then stops capturing altogether.
	Continuous	GSP-830 captures signal when the first triggering condition occurs, then switches to Free Run mode; continues capturing all input signals regardless of their conditions.

Set trigger delay

Background	Trigger delay sets the amount of time between the moment of trigger condition and when GSP-830 starts capturing signal.	
Panel operation	1. Press the Trigger key.	
	2. Press F4 (Trigger Delay).	
	3. Enter the delay time using the numerical keys.	
Delay range	0, 10us ~ 100s, 1us resolution	



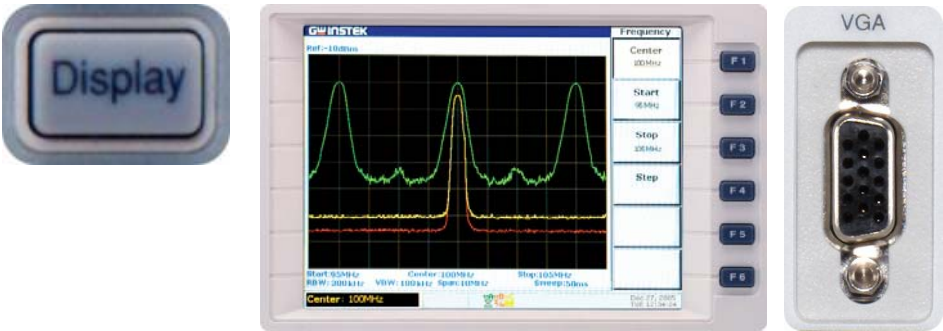


# DISPLAY

**Display** setting configures the LCD screen dimmer level and display layout, including display line, title, and split window. Display line provides a convenient reference line for measuring amplitude. Split window allows two simultaneous waveforms shown on the display. The VGA terminal on the rear panel outputs the LCD screen contents in 640x480 resolution.




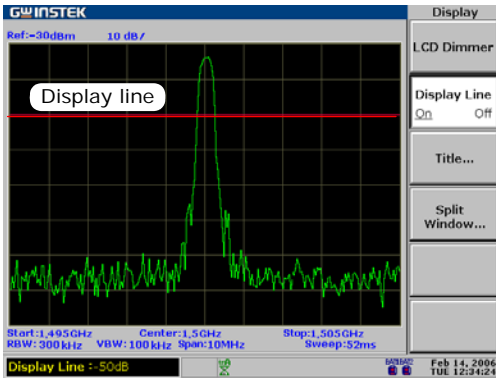





LCD Dimmer	Change Display Brightness.....	111
Display line	Activate Display Line.....	111
Title	Enter Display Title.....	112
Split window	Use Split Display .....	113
VGA output	Use VGA Output .....	114
Save	Save Display Image to USB Flash Drive.....	114

## Change Display Brightness






















Panel operation	1. Press the Display key.	
	2. Press F1 (LCD Dimmer).	 
	3. Change the brightness using the Left/Right key or Scroll knob.	 
Range	0 (darkest) ~ 5 (brightest)	

## Activate Display Line

Panel operation	1. Press the Display key.	
	2. Press F2 (Display Line On).	 
	3. The line appears on the display.	
		
	4. The display line level appears in the command window.	
	5. Move the line using the Arrow key or Scroll knob.	 

Note	Display line is NOT available when the display splits.	
	<ul style="list-style-type: none"> <li>• Split window (page113)</li> <li>• Limit Line editing (page93)</li> <li>• Power measurements (page84)</li> </ul>	

## Enter Display Title

Panel operation	1. Press the Display key.	
	2. Press F2 (Title).	 
	3. Select the character from F2 ~ F4 and press it.	     
	4. Here is how to type in the capital letter "S". Press F2 (Capital Letter) repeatedly until the cursor reaches S.	  
	5. Press the Enter key. S appears in the command window.	  
	6. Continue the above until all the characters are entered.	 (SATEST)
	7. Press F5 (Show Title).	 
	8. The entered title appears at the top left corner of the display.	
	9. To erase the title, press F1 (Clear Title).	 
Parameter	Capital letter	Upper case alphabet, A to Z.
	Small letter	Lower case alphabet, a to z.
	Symbol	Commonly used 14 symbols as shown below.
		<div> \    #    /    _    - </div> <div> .    *    :    &amp;    ( </div> <div> )    &lt;    &gt;    % </div>




# Use Split Display

Panel operation

1. Press the Display key.

Display
2. Press F4 (Split Window).

Split Window...F 4
3. The display splits into upper and lower screen. The lower display retains the original vertical and horizontal scale. The upper display shows full scale.

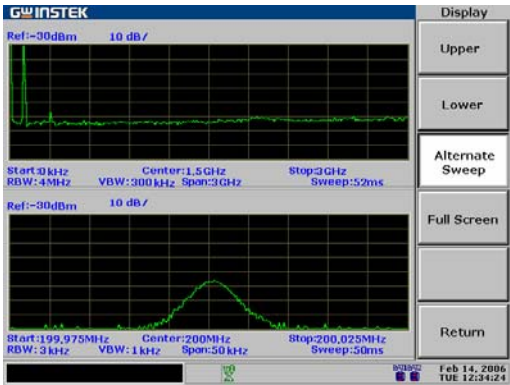

4. Select the active display (the waveform is updated) by pressing F1 (Upper) or F2 (Lower). Pressing F3 (Alternate Sweep) updates both displays alternately.

UpperF 1


LowerF 2

Alternate SweepF 3
5. To go back to the original single display, press F4 (Full Screen). The currently active window gets expanded.

Full ScreenF 4
- \* Switching to Full Screen from the Alternate Sweep mode is not recommended, since it is not predictable which display, upper or lower, will be selected.

# Use VGA Output

Panel operation      Connect an external monitor to rear panel VGA output terminal. The output is always On.



Parameter	Connector type	VGA 15pin, female
	Resolution	640 x 480

# Save Display Image to USB Flash Drive

Panel operation      1. Connect the USB flash drive to front panel USB terminal.



Compatibility	USB 1.1/2.0
Connector	TypeA host, female


2. Press the File key.




3. Press F4 (Print Screen).



4. Press F1 (To Ext. Memory).



5. The USB flash drive contents appear in the window.

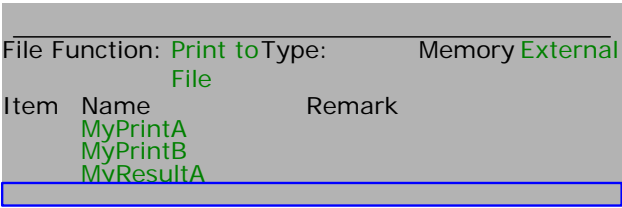

6. To save the display image, press F2 (Print Now). A new \*.bmp file is created in the USB flash drive.



File Function: Print to Type: Memory External

File

Item	Name	Remark
	MyPrintA	
	MyPrintB	
	MvResultA	
	MyFigure	

7. If you want to edit the file name, press F1 (Edit File Name).

Edit File Name

F 1

8. The character table appears at the bottom of the display. Move the cursor inside the table using the Left/Right key and Scroll knob. Press the Enter key to confirm the character.

kHz / μSec

Enter

Char Table

ABCDEFGHIJKLMN O P Q R S T U V W X Y Z a b c d e f

g h i j k l m n o p q r s t u v w x y z 0 1 2 3 4 5 6 7 8 9

9. When completed, press F1 (Edit File Name) again. The file name is confirmed.

Edit File Name

F 1

# FILE

**File** function manages file operations; copy, delete, and name change. The file format and contents include trace waveform, limit line, amplitude correction, sequence set (user defined macro), and panel setup. The file source and destination are selectable between internal and external (USB flash drive). File function also saves display image to USB flash drive.



---



File operation	File Location and File Type.....	117
	File Copy Step.....	118
	File Delete Step.....	121
	File Rename Step.....	123

---

Display image operation	Save Display Image to USB Flash Drive.....	124
-------------------------	--	-----

---

# File Location and File Type

File location	Internal	The GSP-830 internal memory. The number of file is fixed (see below).
	External	The USB flash drive connected to the front panel terminal. There is no practical limit on the number of files.
		
	 The USB icon turns On when the flash drive is detected.	
		Compatibility: USB 1.1/2.0
		Connector: TypeA host, female
File type	Trace	Trace waveform data. For details, see page75. File format: *.tra 13 files are available internally: Trace A/B/C (current trace), Trace 1~10 (stored trace).
	Limit	Limit Line data. For details, see page92. File format: *.lmt 12 files are available internally: LimitHL (current high limit line), LimitHL1~5 (stored high limit line), LimitLL (current low limit line), LimitLL1~5 (stored low limit line).
	Correction	Amplitude correction data. For details, see page53. File format: *.cor 5 files are available: Correction 1 ~ 5.
	Seq.	Sequence data. For details, see page139. File format: *.seq 10 files are available: Sequence 1 ~ 10.

Setup Panel setup data. For details, see page128.  
File format: \*.set  
10 files are available: Setup 1 ~ 10.

## File Copy Step

1. Connect USB flash drive (for external file) When using the USB flash drive (external file) for source or destination, connect the drive to front panel terminal.




The USB icon turns On when the flash drive is detected.

### 2. Select source file

1. Press the File key.




2. Press F1 (Copy).



F 1


3. Press F1 (Source). The source file copy window appears.




F 1

Source		
File Function:	Copy	Type: Memory
Item	Name	Remark


4. Select the file type from F1 ~ F5 and press it.  
Then select Int (internal) or Ext (external).  
The display gets updated accordingly. The below example shows Trace file, internal.




F 1




F 2



F 3




F 4



F 5

Source		
File Function:	Copy	Type: Memory
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	

5. Use the Up/Down key to move the cursor to the copy source file location. (Example: TraceC selected)
- 

Source		
File Function: Copy		Type: Memory
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	

6. Press F6 (Return). The copy source file information is retained.




3. Select destination file

1. Press F2 (Destination). The destination file copy window becomes active (lower half of the display). File type is automatically selected according to the previous Copy source file type selection.



Source		
File Function: Copy		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	
	Trace2	
	Trace3	

Destination		
File Function: Copy		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	
	Trace2	
	Trace3	

2. Use the Up/Down key to move the cursor to the copy destination file location. (Example: Trace1 selected)
- 

Destination		
File Function: Copy		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	

- Press F6 (Return). The copy destination file information is retained.

Return

F 6

#### 4. Copy file

- The copy source and destination files are highlighted (Example: source – TraceC, destination – Trace1)

Source		
File Function: Copy		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	
	Trace2	
	Trace3	

Destination		
File Function: Copy		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	
	Trace2	
	Trace3	

- Press F4 (Copy Now).

Copy Now

F 4

- If the destination file attribute (Remark) has been empty, it changes into full.

Destination		
File Function: Copy		Type: Memory Internal
Item	Name	Remark
	TraceA	empty
	TraceB	empty
	TraceC	empty
	Trace1	full

#### 5. Edit file name (external file, if necessary)


- Move the cursor to the file using the Up/Down key.
- Press F3 (Edit File Name).



Edit File Name

F 3

- The character table appears at the bottom of the display. Move the cursor inside the table using the Left/Right key and Scroll knob. Press the Enter key to confirm the character.






Char Table																									
A	B	C	D	E	F	G	H	I	J	K	L	M	N	O	P	Q	R	S	T	U	V	W	X	Y	Z
a	b	c	d	e	f	g	h	i	j	k	l	m	n	o	p	q	r	s	t	u	v	w	x	y	z
0	1	2	3	4	5	6	7	8	9																

4. When completed, press F3 (Edit File Name) again. The file name is confirmed.
- Edit File Name

F 3

## File Delete Step

1. Connect USB flash drive (for external file)
- When using the USB flash drive (external file) for source or destination, connect the drive to front panel terminal.
- 

 The USB icon turns On when the flash drive is detected.

2. Select source file
1. Press the File key.
- File
2. Press F2 (Delete).
- Delete...

F 2
3. Press F1 (Type). The file deletion window appears.
- Type...

F 1
- | Source                |      |              |
|-----------------------|------|--------------|
| File Function: Delete |      | Type: Memory |
| Item                  | Name | Remark       |
4. Select the file type from F1 ~ F5 and press it.
- Trace

Int. Ext.

F 1
- Then select Int (internal) or Ext (external).
- Limit

Int. Ext.

F 2
- The display gets updated accordingly. The below example shows Trace file, internal.
- Correction

Int. Ext.

F 3
- Seq.

Int. Ext.

F 4
- Setup

Int. Ext.

F 5

Source		
File Function: Delete		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	

5. Use the Up/Down key to move the cursor to the file location.  
(Example: Trace1 selected)



Source		
File Function: Delete		Type: Memory Internal
Item	Name	Remark
	TraceA	
	TraceB	
	TraceC	
	Trace1	

6. Press F6 (Return). The file location is retained.

Return

F 6

### 3. Delete file

1. Press F2 (Delete Now).















Delete Now

F 2

2. Internal file: the file attribute (Remark) changes into Empty.  
In case of external file, the file itself is deleted.

Source		
File Function: Delete		Type: Memory Internal
Item	Name	Remark
	TraceA	full
	TraceB	full
	TraceC	full
	Trace1	empty

# File Rename Step

Background	File rename is allowed only for external (USB flash drive) file. Rename operation is also available during file copy (page118) and display image save (page124).	
1. Connect USB flash drive	When using the USB flash drive (external file) for source or destination, connect the drive to front panel terminal.	
	 The USB icon turns On when the flash drive is detected.	
2. Select file	1. Press the File key.	
	2. Press F3 (Rename). The USB flash drive contents appear on the display.	 
	3. Move the cursor to the file using the Up/Down key.	
	4. Press F3 (Edit File Name).	 
	5. The character table appears at the bottom of the display. Move the cursor inside the table using the Left/Right key and Scroll knob. Press the Enter key to confirm the character.	  
		
	6. When completed, press F2 (Confirm). The file name is confirmed.	 

## Save Display Image to USB Flash Drive

### Panel operation

1. Connect the USB flash drive to front panel USB terminal.




The USB icon turns On when the flash drive is detected.

2. Press the File key.




3. Press F4 (Print Screen).




F 4

4. Press F2 (To Ext. Memory).



F 1


5. The USB flash drive contents appear in the window.

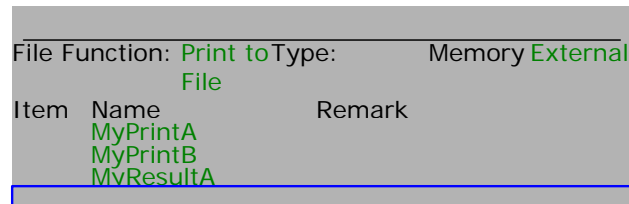


6. To save the display image, press F2 (Print Now). A new \*.bmp file is created in the USB flash drive.



F 2

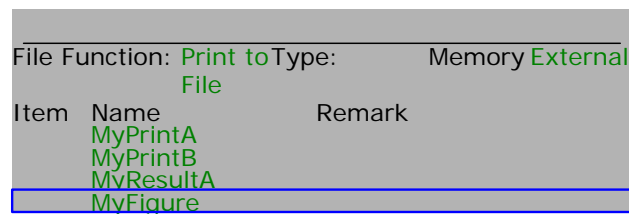


7. If you want to edit the file name, press F1 (Edit File Name).




F 1

8. The character table appears at the bottom of the display. Move the cursor inside the table using the Left/Right key and Scroll knob. Press the Enter key to confirm the character.



Char Table																									
A	B	C	D	E	F	G	H	I	J	K	L	M	N	O	P	Q	R	S	T	U	V	W	X	Y	Z
a	b	c	d	e	f	g	h	i	j	k	l	m	n	o	p	q	r	s	t	u	v	w	x	y	z
0	1	2	3	4	5	6	7	8	9																

9. When completed, press F1 (Edit File Name) again. The file name is confirmed.



# PRESET






Pressing the Preset key brings back GSP-830 to the below state. The same content is also shown in page41.

Frequency	Center: 1.5GHz Start: 0Hz	Stop: 3GHz Step: 1MHz
Span	3GHz	
Amplitude	Ref.level: 0dBm Unit: dBm Correction: Off	Scale: 10dB/ External Gain: 0dB Input Z: 50Ω
Autoset	Amplitude Floor: Auto	Span: Auto
Marker	Marker: Off Marker Table: Off	Marker Trace: Auto All Marker: Off
Peak Search	Peak Table: Off Peak Threshold: Off	Peak Sort: Freq Peak Track: Off
Trace	Trace: A AVG: Off	Mode: Clear Detection: Normal
Meas	ACPR, OCBW: Off CH SPC: 0 CH BW: 600MHz OCBW %: 0	N dB, Phase Jitter: Off Adj CH Offs1: 600MHz Adj CH Offs2: 1200MHz Adj CH BW1&2: 600MHz
Limit Line	H & L Limit: Off	Pass/ Fail: Off
BW	RBW, VBW, Swptime: Auto	Average: Off
Trigger	Trigger Delay: 50ms Trigger Mode: Normal	Trigger Freq: 1.5GHz
Display	LCD Dimmer: 5 Split Window Lower: Off	Display Line: Off Split Window Upper: Off
File	Copy Type: Int. Trace	Delete Type: Int. Trace
System	GPIO Add: 2 Aux Sig: Off	System Config: Off Language: English
Option	External Ref Freq: 10MHz TG Norm Corr: Off Demod AM: Off	TG Output: Off TG Ref Value: 0dBm Demod FM: Off
Sequence	Sequence: 1	Run Mode: Single












# S SYSTEM

**System key** configures and displays the system settings, including self-test result, date/time setting, and synchronization with other devices. The panel setting can be saved into file and recalled later, even in other GSP-830s.

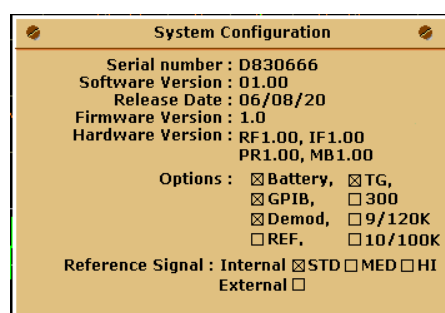








Panel setting	Save/Recall Panel Setting .....	128
	Copy/delete/rename setup .....	128
Interface configuration	USB slave port configuration .....	129
	RS-232C configuration.....	129
	GPIB configuration (optional) .....	130
System information	View system error.....	131
	View system configuration .....	132
	View self-test result .....	134
Date/Time	Set Date/Time.....	135
Synchronization	GSP as a master (internal reference signal).....	136
	GSP as a slave (external reference signal) .....	137
Language	Select Menu Language .....	138
Service operation	Service operation menu.....	138

## Save/Recall Panel Setting








Panel operation	1. Press the System key.	
	2. Press F1 (Save/Recall Setup).	 
	3. Press F1 or F2 repeatedly to select the setup file.	   
	4. Press F3 (Save Now) or F4 (Recall Now) to save or recall the panel setup file.	   
File contents	Setup file contains the following information. <ul style="list-style-type: none"> <li>• Reference amplitude level</li> <li>• Amplitude unit, scale</li> <li>• Start/stop frequencies</li> <li>• Center and span frequencies</li> <li>• VBW, RBW, and sweep time</li> <li>• Tracking Generator level</li> <li>• Tracking Generator normalization data</li> </ul>	

## Copy/delete/rename setup file


Background	Setup files can be copied, deleted, or renamed using the file utility. Press the File key to access each function.	
Copy	Press F1 (Copy). For detailed step, see page118.	 
Delete	Press F2 (Delete). For detailed step, see page121.	 
Rename	Press F3 (Rename). For detailed step, see page123.	 



## Configure Communication Interface

Background	Communication interface is used in the following occasions. The interface configuration is introduced in the relevant chapter too.	
	PC software (page153)	USB slave, RS-232C
	Remote control (page161)	USB slave, RS-232C, GPIB (optional)
Interface type	USB slave	USB 1.1 or 2.0, TypeB mini, female connector. Used in PC software connection and remote control.
	RS-232C	D-sub 9 pin, female connector. Used in PC software connection and remote control.
	GPIB (optional)	24pin female connector. Used in remote control.
USB slave port configuration	No need for panel configuration: Just connect a USB cable to the rear panel. Type B mini, female, USB1.1/2.0	
RS-232C configuration	1. The RS-232C configuration can be checked from the system menu. Press the System key.	
	2. Press F3 (Serial Port).	
	3. The RS-232C port configuration appears. Configure the PC according to this setting. Baud: 115200 Parity: None Stop bit: 1 Data bit: 8	   


4. Connect RS-232C cable to the rear panel terminal.  
9 pin, female



GPIB configuration  
(optional)

GPIB interface is a factory installed optional item.  
Contact service personnel for a new installation.

1. Press the System key.




2. Press F2 (GPIB Add).



3. Select GPIB address using the Arrow key or Scroll knob.  
Configure the PC according to this setting.




4. Connect GPIB cable to the rear panel terminal.



Check GPIB installation status

1. To check the GPIB installation status, press the System key.



2. Press F6 (More).



3. Press F4 (System Config).




4. The system configuration window appears. When the GPIB module is installed correctly, the check box is marked.




Check GPIB self-test result

1. To check the internal GPIB functionality result, press the System key.



2. Press F6 (More).



3. Press F2 (Self Test).

Self Test...

F 2
4. The GPIB result appears at F1.  
If the result is Fail (underlined),  
contact service personnel.

GPIB

Pass Fail

F 1

GPIB constraints

Keep these rules when using GPIB interface.

- Altogether less than 15 devices & 20m cable length, 2m between each device on the bus
- Unique address assigned for each device
- At least 2/3 of the GPIB devices turned On
- No loop or parallel structure allowed

## View System Information

### View system error

Panel operation

View the bottom of the screen, the error message area.  
If there is a system error, the message appears in red color.

Center : 1.5GHz

EXT  
Unlock

(EXT Unlock)

Here is the error list.

EXT  
Unlock

External reference input is not working properly.

Ref  
Unlock

Internal reference signal is not working properly.






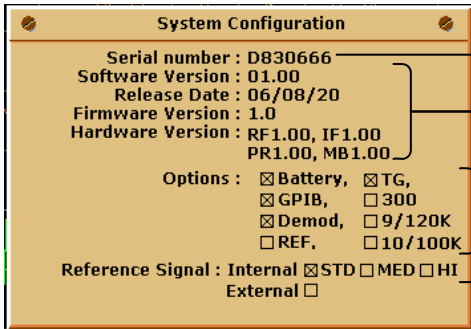



LO1  
Unlock

Local oscillator 1 is not working properly.

LO3  
Unlock

Local oscillator 3 is not working properly.
















View system configuration

Panel operation	1.	To check system configuration, press the System key.	
	2.	Press F6 (More).	 
	3.	Press F4 (System Config On).	 
	4.	The system configuration window appears. Four types of information are listed from the top. <ul style="list-style-type: none"><li>• Serial number</li><li>• Software and hardware version</li><li>• Optional items installation</li><li>• Reference signal selection</li></ul>	
			
	5.	To close the configuration window, press F4 again (System Config Off).	 
Serial number	The serial Number for device identification. This number is necessary for various service level operations. The same number is pasted on the rear panel.		
			
Software/hardware version	Shows versions and release date of hardware, software, and firmware. Used for service level operations.		

Optional item installation status	Shows which optional item is currently installed. <input checked="" type="checkbox"/> : installed, <input type="checkbox"/> : uninstalled.	
	Sign	Description
	<b>Battery</b>	Battery pack / DC input module (page151)
	<b>GPIB</b>	GPIB interface (page130)
	<b>Demod</b>	Demodulator (page147)
	<b>REF</b>	Internal reference signal with middle range stability in $\pm 1$ ppm stability module (page182).
	<b>300</b>	300Hz RBW (page99)
	<b>9/120K</b>	9k/120kHz RBW (page99) included in the EMI Filter (page149)
	<b>10/100K</b>	10k/100kHz RBW (page99)
Reference signal status	Checked radio button shows the reference signal used. For reference signal usage, see page136. <input checked="" type="checkbox"/> : enabled, <input type="checkbox"/> : disabled.	
	Sign	Description
	<b>Internal STD</b>	Internal reference signal, standard stability
	<b>Internal MED</b>	Internal reference signal, medium stability. Available when the $\pm 1$ ppm stability module (page182) is installed.
	<b>Internal HI</b>	Internal reference signal, high stability (reserved).
	<b>External</b>	External reference signal.

## View self-test result


GSP-830 runs a series of internal tests upon power-up.

Background	GSP-830 runs a series of internal tests upon power-up. If any of the test result shows fail, contact service personnel.	
Panel operation	1. Press the System key.	
	2. Press F6 (More).	 
	3. Press F2 (Self Test).	 
	4. The result appears in F1 ~ F4. (The GPIB result appears only when the module is installed)	<div> </div> <div> </div> <div> </div> <div> </div>
	5. Press F6 (Return) to go back to the previous menu.	 
Item	GPIB	The optional GPIB interface connection. Available only when the GPIB module is installed (page132).
	Flash	Internal flash memory area for storing the system code and data.
	SDRAM	Internal SDRAM area on which the code runs.
	RTC	The real-time clock that controls the date and time setting (page135).


## Set Date/Time

### 1. Activate clock display


1. Press the System key.




2. Press F6 (More).



3. Press F1 (System Clock).



- Press F3 (Clock On). The clock appears on the bottom right side of the display.



## 2. Set date




1. Press F1 (Date).



2. Press F1 (Year) ~ F4 (Day of Week). Enter the value using the numerical keys. Press the Enter key to confirm the value.



The clock display changes accordingly.



Year 2000 ~ 2064


Month 1 ~ 12 (translated to Jan ~ Dec)

Day 1 ~ 31

Day of Week 1 ~ 7 (translated to Sun ~ Sat)

### 3. Set time




1. Press F1 (Date).



2. Press F1 (Year) ~ F3 (Second). Enter the value using the numerical keys. Press the Enter key to confirm the value.



The clock display changes accordingly.










Hour	0 ~ 23
Minute	0 ~ 59
Second	0 ~ 59

## Synchronize GSP-830 with Other Device











Using the reference frequency input/output on the rear panel, GSP-830 can synchronize its internal frequency with other device. GSP-830 can become the master (output the reference signal to other device) or the slave (input the reference signal from other device).

### GSP as a master (internal reference signal)








Panel operation	Connect the reference signal output terminal on the rear panel to the other device's reference input.	
Signal type	Output level	10MHz, 5V TTL signal (assuming the load impedance is infinite)
	Output impedance	50Ω
Stability check	1. Press the System key.	
	2. Press F6 (More).	 
	3. Press F4 (System Config On).	 
	The system configuration window appears. The Internal Reference Signal sign <b>Internal</b> shows the status. <input checked="" type="checkbox"/> : enabled, <input type="checkbox"/> : disabled.	
	<b>STD</b>	Internal reference signal, standard stability
	<b>MED</b> 	Internal reference signal, median stability. Available when the ±1ppm stability module (page182) is installed. The MED icon appears at the bottom of the display.
	<b>HI</b>	Internal reference signal, high stability (reserved).



GSP as a slave (external reference signal)










Panel operation	1. Press the Option key.				
	2. Press F4 (Ext Ref Freq) to enable external reference signal.				
	3. Use the Arrow key to select the external reference frequency.				
	4. Connect the external reference signal to the input terminal on the rear panel.				
	5. The external reference signal icon appears at the bottom of the display.				
Frequency	10 types are available (units in MHz).				
	1.0	1.544	2.048	5.0	10.0
	10.24	13.0	15.36	15.4	19.2
Status check	1. Press the System key.				
	2. Press F6 (More).				
	3. Press F4 (System Config On).				
The system configuration window appears. The External Reference Signal sign <b>External</b> shows the status.  : enabled,  : disabled.					

## Select Menu Language

Panel operation	1. Press the System key.	
	2. Press F6 (More).	 
	3. Press F5 (Language).	 
	4. Press F1 repeatedly to select the menu language.	 
Language type	English → Simplified Chinese → Other selections (differs according to the region) → English	


## Service operation menu

The following functions are intended only for service personnel.

Optional items maintenance	1. Press the System key.	
	2. Press F5 (Service).	 
	3. In order to continue, you need to type in the password into the command window.	
RF diagnosis	1. Press the System key.	
	2. Press F6 (More).	 
	3. Press F3 (RF Diagno) to see the RF diagnosis result.	 






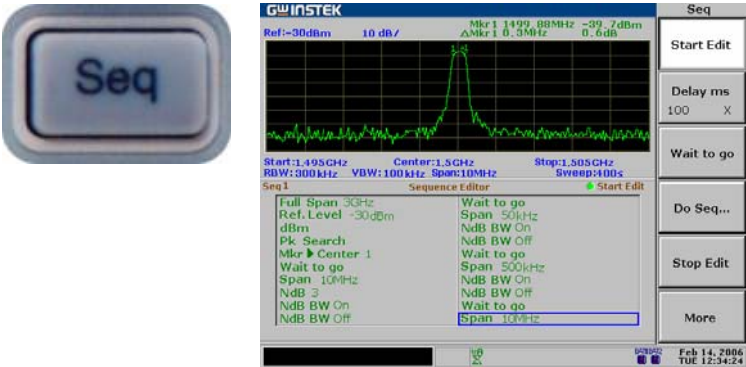











# SEQUENCE




Sequence function records and playbacks user-defined macro (measurement steps). 10 sequences are available in repeat or single running mode, each with 20 steps available for all panel operations. Delay and pause features allows observing measurement result during the sequence.














Edit	1. Select sequence .....	140
	2. Start editing.....	140
	3. Stop editing.....	143
	4. Save the edited sequence .....	143
	Delete all sequence .....	143
Run	1. Select sequence .....	143
	2. Select running mode .....	144
	3. Run sequence.....	144
Sequence File	Save/copy/delete/rename sequence file .....	144

## Edit Sequence

1. Select sequence	1. Press the Sequence key.	
	2. Press F1 (sequence 1 ~ 5) or F2 (sequence 6 ~ 10) repeatedly to select the sequence ID.	 
2. Start editing	1. Press F3 (Edit).	 
	2. Press F1 (Start Edit).	 
	3. The Start Edit sign on the middle of the display turns green.	
2a. Add step	20 steps are available for each sequence. Every key operation can be recorded as a step. Press the Enter key each time to confirm step entering. (In some cases this is not necessary: check if the item appears in the window).	
	Example: Activate system auxiliary signal	
	1. Press the System key.	
	2. Press F4 (Aux Sig On).	 
	3. Press the Enter key.	
	Example: Run Autoset	
	1. Press the Autoset key.	
	2. Press F1 (Autoset).	 
	3. Press the Enter key.	
	The result looks like this.	

2b. Add delay	The delay function inserts a waiting period between steps.
1. Press F2 (Delay ms).	<div>Delay ms</div> <div>100 X</div> <div>F 2</div>
2. Enter the time of delay period (100ms) insertion using the numerical keys. For example, pressing 5 times inserts 500ms (5 * 100ms).	
Range	1 ~ 100, 100ms resolution
2c. Pause sequence	Stops executing the sequence until the user press F1 (Continue). Useful for observing the result of particular action (for example ACPR measurement).
1. Press F3 (Wait to go).	<div>Wait to go</div> <div>F 3</div>
2. When the sequence is running, F1 (Continue) menu appears on the menu.	<div>Continue</div> <div>F 1</div>
2d. Insert another sequence	Inserts a whole sequence set.
1. Press F4 (Do Seq).	<div>Do Seq...</div> <div>F 4</div>
2. Press F1 (sequence 1 ~ 5) or F2 (sequence 6 ~ 10) repeatedly to select the inserted sequence.	<div>Select Seq</div> <div>1 2 3 4 5</div> <div>F 1</div> <div>Select Seq</div> <div>6 7 8 9 10</div> <div>F 2</div> 
Note	You cannot insert the currently edited sequence.
2e. Insert blank space	1. Press F6 (More).
	<div>More</div> <div>F 6</div>
	2. Use the Up/Down key to move the cursor to the insertion point.
	
	3. Press F1 (Insert). A new blank space will be created.
	<div>Insert</div> <div>F 1</div>

		  
	4. Press F6 (Return) to go back to the previous menu.	<div>Return</div> <div>F 6</div>
2f. Delete step	1. Press F6 (More).	<div>More</div> <div>F 6</div>
	2. Use the Up/Down key to move the cursor to the deletion point.	
	3. Press F3 (Delete). The step will be deleted.	<div>Delete</div> <div>F 3</div>
		  
	4. To undo deletion, press F5 (Undelete).	<div>Undelete</div> <div>F 5</div>
	5. To go back to the previous menu, press F6 (Return).	<div>Return</div> <div>F 6</div>
2g. Delete all steps in a sequence	1. Press F6 (More).	<div>More</div> <div>F 6</div>
	2. Press F4 (Delete All).	<div>Delete All..</div> <div>F 4</div>
	3. Press F2 (Yes) to confirm, or F1 (No) to cancel. All steps will be deleted.	<div>No</div> <div>F 1</div>
		<div>Yes</div> <div>F 2</div>
		  
	4. To undo deletion, press F5 (Undelete).	<div>Undelete</div> <div>F 5</div>

3. Stop editing	5. Press F6 (Return) to go back to the previous menu.	Return	F 6
	1. Press F5 (Stop Edit).	Stop Edit	F 5
	2. The Start Edit sign on the middle of the display turns gray.		
4. Save the edited sequence	1. Press F6 (More).	More	F 6
	2. Press F2 (Save). The sequence is saved.	Save	F 2
	3. Press F6 (Return) to go back to the previous menu.	Return	F 6

Delete all sequences


Panel operation	1. Press the Sequence key.	Seq	
	2. Press F5 (Delete Seq All).	Delete Seq All...	F 5
	3. Press F2 (Yes) to confirm, or F1 (No) to cancel. All 10 sequences will be deleted.	No	F 1
		Yes	F 2
	4. To go back to the previous menu, press F6 (Return).	Return	F 6

Note	Delete Seq All cannot be recovered – the Undelete function is not applicable.
------	---

Run Sequence

This section assumes that the sequence is already edited.

1. Select sequence	1. Press the Sequence key	Seq	
	2. Press F1 (sequence 1 ~ 5) or F2 (sequence 6 ~ 10) repeatedly to select the sequence.	<div>Select Seq 1 2 3 4 5</div> <div>Select Seq 6 7 8 9 10</div>	<div>F 1</div> <div>F 2</div>

2. Select running mode	1. Press F4 (Run).	Run...	F 4
	2. Press F1 (Run Mode) to select the running mode, repeat (Rept) or single (Sngl).	Run Mode Rept Sngl	F 1
	Repeat	Repeats running a sequence until F6 (Stop) is pressed. Note: F6 (Stop) menu appears only when the sequence is running.	
	Single	Runs the sequence once.	
3. Run sequence	1. Press F2 (Run Now).	Run Now	F 2
	2. The sequence icon appears at the bottom of the display.		
	3. To stop running, press F6 (Stop). In the single mode, the sequence automatically stops when all steps are completed.	Stop	F 6

### Save/copy/delete/rename sequence file

Background	Sequence files can be saved, copied, deleted, or renamed using the file utility. Press the File key to access each function.	File	
Save/Copy	Press F1 (Copy). For detailed step, see page118.	Copy...	F 1
Delete	Press F2 (Delete). For detailed step, see page121.	Delete...	F 2
Rename	Press F3 (Rename). For detailed step, see page123.	Rename...	F 3












# T

## RACKING GENERATOR



















The optional **Tracking Generator** generates a sweep signal with its sweep time and its frequency range matching the GSP-830 system. The amplitude is maintained to a constant value over the entire frequency range, which is very useful for testing the frequency response of the Device Under Test.










### Activate tracking generator

1. Activate TG output	1. Press the Option key.	
	2. Press F1 (TG).	 
	3. Press F1 (TG On).	 
	4. The tracking generator output becomes activated.	
2. Set TG output level	1. Press F2 (TG Level).	 
	2. Change the TG output level using the Arrow key and Scroll knob.	
Range		0 ~ -50dBm

## Normalize tracking generator

1. Set reference level	1. Press the Option key.		
	2. Press F1 (TG).		
	3. Press F5 (Ref Value).		
	4. Set the reference value using the Arrow key or Scroll knob.  Normalization target level is set at Reference value, regardless of the TG output level.  Range      -130 ~ +20dBm	 	
2. Run normalization	1. Press F3 (Execute Normalization).		
	2. Press F2 (Yes) to confirm, or F1 (No) to cancel. Normalization runs.	 	 
	3. Press F6 (Return) to go back to the previous menu.		
3. Activate normalization	1. To enable normalization, press F4 (Norm Corr On).		
	2. Normalization is activated and the TG icon appears.		

## Check TG installation status

1. Run normalization	1. Press the System key.		
	2. Press F6 (More).		
	3. Press F4 (System Config On). The configuration appears.		
	4. The TG sign shows the installation status, installed (checked) or not installed (unchecked).	Installed  Not installed 	

# DEMODULATOR

The optional FM/AM **Demodulator** recovers AM or FM modulated baseband signal. The demodulated signal can be output from the rear panel mono phone jack.



## Activate Demodulation







Panel operation	1. Press the Option key.	
	2. Press F2 (Demod).	
	3. Select Frequency Modulation or Amplitude Modulation by pressing F1 (FM On) or F2 (AM On).	 

## Activate phone output







Panel operation	1. Press F2 (Demod).	
	2. Press F3 (SPK On).	
	3. The rear panel phone output becomes active. 3.5mm, mono (stereo plug)	

Note	The FM or AM must be activated before SPK On.
------	---






## Set phone output volume

Panel operation	1. Press F2 (Demod).		
	2. Press F4 (Volume).		
	3. The volume level appears in the command window.		
	4. Change the output volume using the Numerical keys, Arrow key, or Scroll knob.		
Volume level	0 ~ 63		

## Cut off phone output noise (squelch)

Panel operation	1. Press F2 (Demod).		
	2. Press F5 (Squelch).		
	3. The squelch level appears in the command window. Output level lower than the setting is muted.		
	4. Change the squelch level using the Numerical keys, Arrow key, or Scroll knob.		
Squelch level	0 ~ 4		

## Check Demodulator installation status

Panel operation	1. Press the System key.		
	2. Press F6 (More).		
	3. Press F4 (System Config On). The configuration appears.		
	4. The Demodulator sign shows the installation status, installed (checked) or not installed (unchecked).	Installed <input checked="" type="checkbox"/> Demod Not installed <input type="checkbox"/> Demod	




# EMI FILTER

The optional **EMI filter** is used for specific measurement situations such as EMI average detection, where higher level of sensitivity is required than the standard configuration. When this module is installed, GSP-830 gets two additional features: Average/Quasi-peak detection mode, and 9k/120k RBW. For a new installation, contact the service center.

## Select AVG/ QPeak signal detection mode





Panel operation	1. Press the Trace key.	<div>Trace</div>	
	2. Press F6 (More).	<div>More</div>	<div>F 6</div>
	3. Press F3 (Detection).	<div>Detection..</div>	<div>F 3</div>
	4. The signal detection mode appears. When the EMI filter is installed, F4 (AVG) and F5 (QPeak) becomes available. For signal detection mode details, see page82.	<div>Normal</div>	<div>F 1</div>
		<div>Sample</div>	<div>F 2</div>
		<div>Peak+</div>	<div>F 3</div>
<div>AVG</div>		<div>F 4</div>	
	<div>QPeak</div>	<div>F 5</div>	
Parameter	AVG (average)	Detects the average power level of the samples using a low pass filter. Useful for smoothing the noise level.	
	QPeak (quasi-peak)	Detects the quasi-peak power level of the samples. Useful for viewing in zero span without missing signal variations.	

## Select 9kHz/120kHz RBW

Panel operation	1. Press the BW key.	
	2. Press F1 (RBW Manu).	
	3. Select 9kHz/120kHz RBW using the Scroll key. The RBW value appears in the command window.	

Note	In the automatic mode, RBW is selected according to the internal reference setting. For reference RBW/VBW setting, see page102.
------	--

## Check EMI filter installation status

Panel operation	1. Press the System key.	
	2. Press F6 (More).	
	3. Press F4 (System Config On). The system configuration window appears.	
	4. The 9/120k RBW sign shows the installation status, installed (checked) or not installed (unchecked).	

Note	EMI filter (9k/120k RBW) and 10k/100k RBW are exclusive. They cannot be installed together.
------	---

# BATTERY / DC OPERATION

Battery/DC operation kit is an optional item for using GSP-830 in outdoor environment, such as field operation using battery and automobile using DC outlet.



## Battery Operation


Package removal /  
insertion



Turn Off the main power switch before inserting or removing the battery pack.



Take out the battery when not in use for a long time.  
Turn the knob to open the battery compartment.

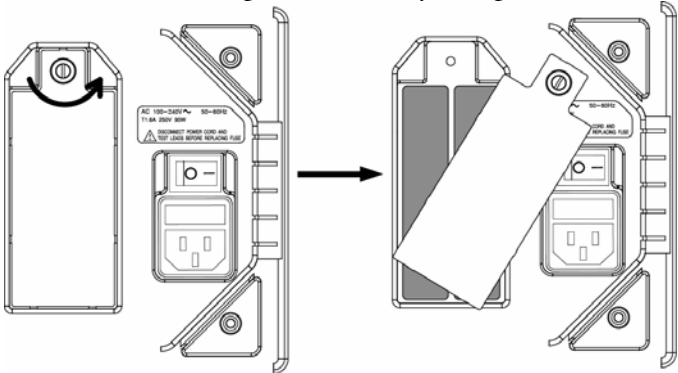


Check Battery level

1. Press the Option key.



	2. Press F3 (Battery). The level icon appears at display bottom.	<div>Battery</div> <div>F 3</div>
	<div>BAT</div> Fully charged	<div>BAT</div> 50% ~ 25%
	<div>BAT</div> 75% ~ 50%	<div>BAT</div> Less than 25%
Note	Regardless of this operation, GSP-830 shows the icon for 5 seconds every 30 minutes.	
Parameter	Usage time	3 hours (typical)
	Charge time	3 hours (typical)

DC Operation

Panel operation	Connect the DC power cable to the rear panel input connector.	<div></div>
Rating	12V, 40W max	<div>DC 12V INPUT 40W MAX.</div>
Note	DC power cable (with lighter plug for automobile usage) is available as another optional item, GTL-401 (page182).	


Check Battery/DC module installation status

Panel operation	1. Press the System key.	<div>System</div>
	2. Press F6 (More).	<div>More...</div> <div>F 6</div>
	3. Press F4 (System Config On). The configuration appears.	<div>System Config On Off</div> <div>F 4</div>
	4. The Battery sign shows the installation status, installed (checked) or not installed (unchecked).	<div>Installed <input checked="" type="checkbox"/> Battery</div> <div>Not installed <input type="checkbox"/> Battery</div>



# PC SOFTWARE

The proprietary PC software for remote operation is downloadable from GoodWill Instruments website. It monitors the waveform and allows panel operations from the familiar PC environment, including large display and keyboard/mouse operation.

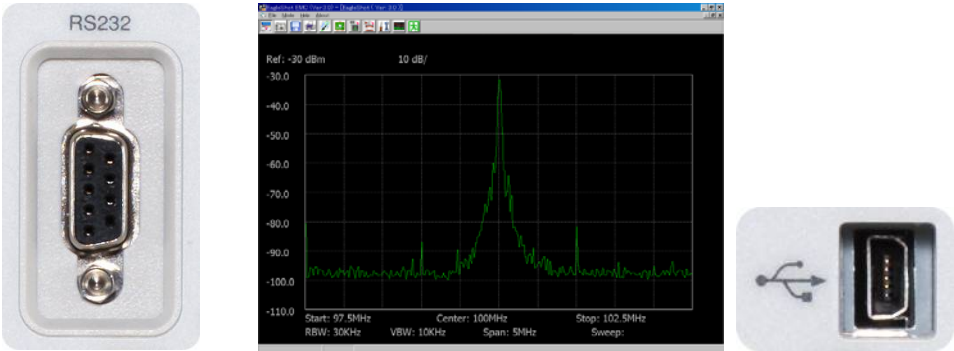

Installation	PC requirement .....	154
	Software download .....	154
	Installation step .....	154
Invocation	Configure interface .....	155
	Invoke software .....	156
Usage	Establish connection .....	158
	Capture waveform .....	158
	Clear waveform .....	158
	Save waveform .....	159
	Printout screen image .....	159
	Use marker .....	159
	Exit program .....	160

## Install Software

### PC requirement

Software	OS	Windows 2000/XP
Hardware	USB	1 USB host connector, 1.1 or 2.0 compatible

### Software download

1. Website access
 

Access <http://www.gwinstek.com.tw/>.  
Click the Download menu on the left task bar.



2. Download page
 

The Software download screen appears. Select Spectrum Analyzer from the drop down menu.




3. Download
 

Click the PC software name under GSP-830 section and download the software package to your local PC.

### Installation step

1. Activate setup software
  1. Unpack the zip file.
  2. Double click Setup.exe.
  3. The setup screen opens. Close all other applications and click OK. If you need to quit setup, press Exit Setup.

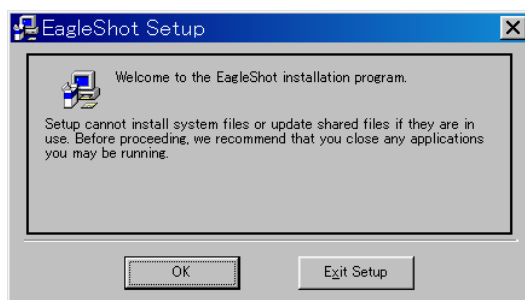


## 2. Start installation


1. If you install to a specific directory, click the Change Directory button.

Change Directory

2. Click the icon to start installation.

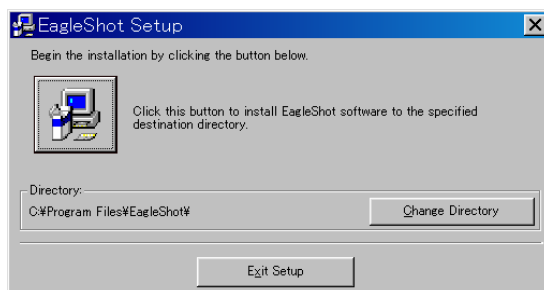

3. When the successful installation message appears, click OK.

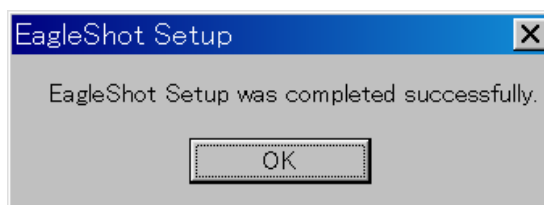

## Connect Software


This section assumes the software is already installed.

### Configure interface

USB slave, or RS-232C is available.


#### Configure USB

No need to configure anything on GSP-830 side. Just connect the USB cable to the rear panel. Type B mini, female connector



#### Configure RS-232C

1. The RS-232C configuration can be checked from the system menu. Press the System key.
2. Press F3 (Serial Port).




Serial Port..

F 3

3. The RS-232C port configuration appears. Configure the PC according to this setting.  
 Baud: 115200  
 Parity: None  
 Stop bit: 1  
 Data bit: 8
 

Baud 115200	F 1
Parity None	F 2
Stop 1	F 3
Data 8	F 4
4. Connect the RS-232C cable to the rear panel terminal.  
 9 pin, female
 




## Invoke software

### PC operation


1. Invoke the software from startup menu.




2. The software opens.

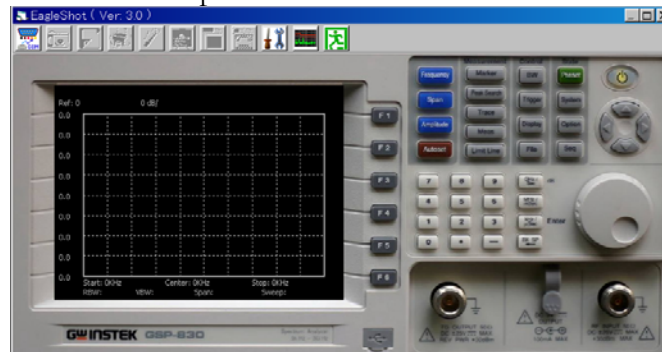

3. Click the setting icon. The parameter setting window appears.

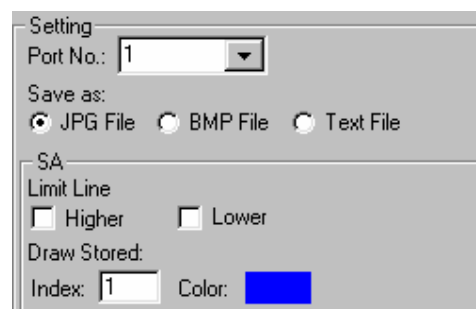

4. Select the connection port (COM port for serial connection)

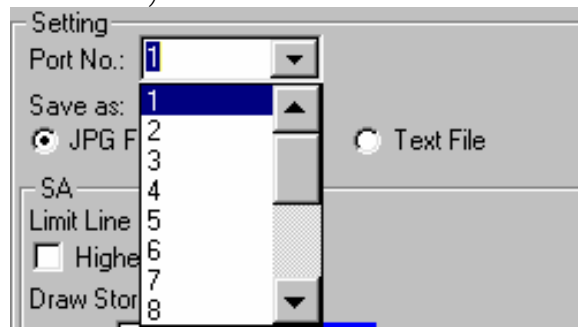

Port selection

Select the port specified in the PC configuration. To check the configuration in PC, go to Control panel → System properties → Hardware tab → Device Manager.

5. Click the Setting icon again to close the setting window




6. Click the Open COM Port icon. The connection is established when the other icons becomes active.






Functionality check

Click the Capture icon. Make sure the waveform shown in GSP-830 display is captured correctly.

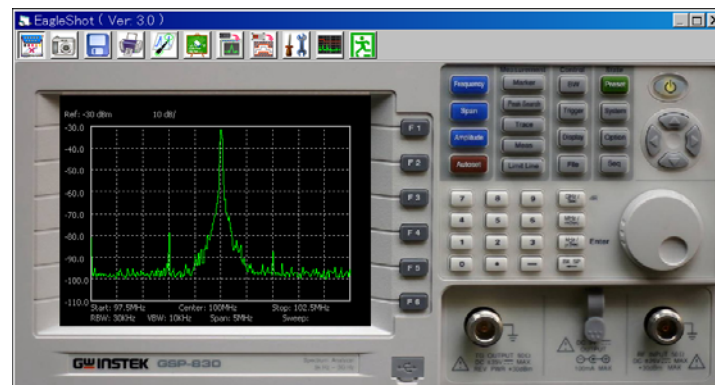


## Use Software


### Establish connection

Operation step	1. Press the setting icon and open the parameter setting window.	
	2. Select the serial port terminal.	
	3. Press the COM port icon. The connection is established when the other icons becomes active.	
Port setting	Select the port specified in the PC configuration. To check the configuration in PC, go to Control panel → System properties → Hardware tab → Device Manager.	


註解 [IK1]:

### Capture waveform


Operation step	Click the capture icon. The current waveform is captured and appears on the screen.	
----------------	---	--

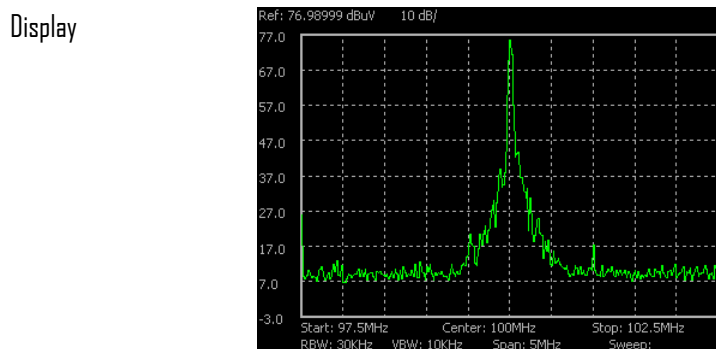

### Clear waveform

Operation step	Click the clear trace icon. The waveform is cleared from the screen.	
----------------	--	---

## Display

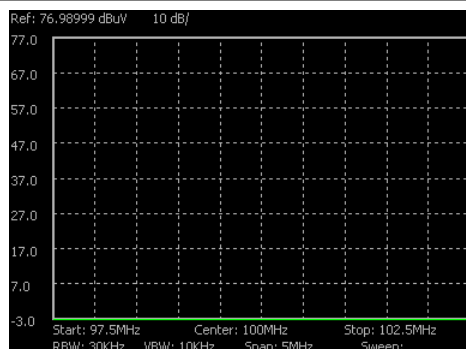

## Save waveform

### Operation step

1. Press the setting icon. Select the file format from \*.jpg/\*.bmp (screen snapshot), \*.txt (measurement data).



Save as:  
☒ JPG File   ☐ BMP File   ☐ Text File

2. Press the save icon. The Windows standard save dialogue window opens. Select the directory and save the file.



### File format

The \*.txt file contains the following information.

- Frequency (MHz) and Amplitude for all waveforms
- Amplitude reference level, unit, and scale
- Start, Stop, Center frequency, and frequency span
- RBW, VBW, and sweep time
- Date and time (if already configured)

## Printout screen image

### Operation step

Click the print icon. The Windows standard printout dialogue opens. Select the printer and printout the screen image.



### Note

The screen image contrast will be reversed (background color becomes white).

## Use marker


### Operation step

1. Click the marker icon. The marker function window appears.



Marker Function

☒ Live ☐ Storage

	Freq(MHz)	Delta
<input checked="" type="checkbox"/> 0	99	
<input checked="" type="checkbox"/> 1	100	0
<input type="checkbox"/> 2	0	N
<input type="checkbox"/> 3	0	N
<input type="checkbox"/> 4	0	N

2. Select Live or Storage.  

3. Check the marker ID box. 5 markers, 0 to 4, are available.

☒ 0  
☒ 1


4. Enter the frequency to each marker.

Freq(MHz)  
99  
100

5. Select normal (N) or delta marker. Example:  
Marker0 & Delta 1: the delta marker shows the difference between marker0 and marker1.

Delta  
  
0  
N

6. The display gets updated with markers in red color and marker values listed on the bottom.

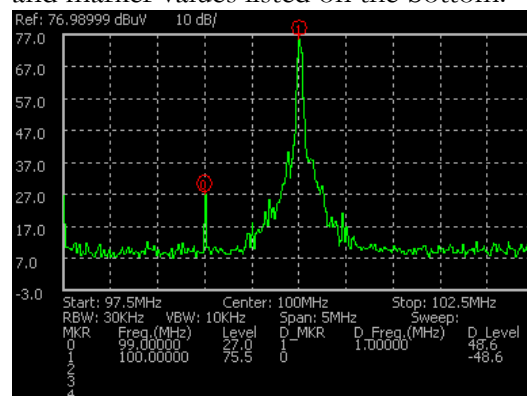

## Exit program

Operation step


Click the exit icon or press Alt key + F4.






















# REMOTE CONTROL

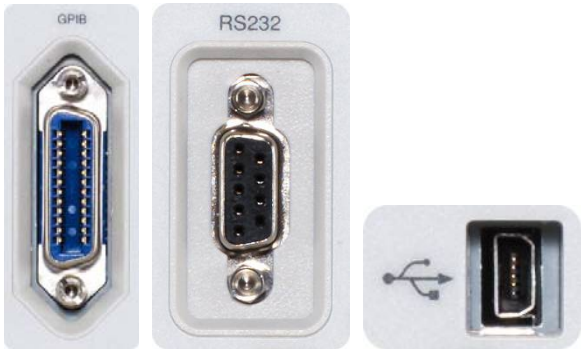GSP-830 supports remote control which is partially based on IEEE 488.2 and SCPI standard. The command set covers most of the panel operations. Three interfaces are available: USB slave, RS-232, and GPIB (optional).



Interface	Configure Interface.....	162
Command Syntax	Command Syntax.....	164
Command Set	Command Set.....	165

## Configure Interface


Interface type	USB slave	USB 1.1 or 2.0, TypeB mini, female connector.
	RS-232C	D-sub 9 pin, female connector.
	GPIO (optional)	24pin female connector.
USB slave port configuration	<p>No need for panel configuration: Just connect a USB cable to the rear panel. Type B mini, female, USB1.1/2.0</p> <p> The USB icon turns On when the connection is detected.</p> 	
RS-232C configuration	1. The RS-232C configuration can be checked from the system menu. Press the System key.	
	2. Press F3 (Serial Port).	 
	3. The RS-232C port configuration appears. Configure the PC according to this setting: Baud: 115200 Parity: None Stop bit: 1 Data bit: 8	       
	4. Connect the RS-232C cable to the rear panel terminal. 9 pin, female	
GPIO (optional) configuration	GPIO interface is a factory installed optional item. Contact the service center for a new installation.	
	1. Press the System key.	
	2. Press F2 (GPIO Add).	 

	<div>3. Select the GPIB address using the Left/Right key or Scroll knob. Configure the PC accordingly.</div>	<div><div><div></div></div><div></div></div>
	<div>4. Connect the GPIB cable to the rear panel terminal.</div>	<div><div></div></div>
Check GPIB installation status	<div>1. To check the GPIB installation status, press the System key.</div>	<div><div>System</div></div>
	<div>2. Press F6 (More).</div>	<div><div>More...</div><div>F 6</div></div>
	<div>3. Press F4 (System Config).</div>	<div><div>System Config On Off</div><div>F 4</div></div>
	<div>4. The system configuration window appears. GPIB sign shows installed (checked) or not installed (unchecked)</div>	<div><div>Installed <input checked="" type="checkbox"/> GPIB Not installed <input type="checkbox"/> GPIB</div></div>
Check GPIB self-test result	<div>1. To check the internal GPIB functionality test result, press the System key.</div>	<div><div>System</div></div>
	<div>2. Press F6 (More).</div>	<div><div>More...</div><div>F 6</div></div>
	<div>3. Press F2 (Self Test).</div>	<div><div>Self Test...</div><div>F 2</div></div>
	<div>4. The GPIB result appears at F1. If the result is Fail (underlined), contact the service center.</div>	<div><div>GPIB <u>Pass</u> Fail</div><div>F 1</div></div>
GPIB constraints	<div>Keep these rules when using the GPIB interface.<ul style="list-style-type: none"><li>• Altogether less than 15 devices &amp; 20m cable length, 2m between each device on the bus</li><li>• Unique address assigned for each device</li><li>• At least 2/3 of the GPIB devices turned On</li><li>• No loop or parallel structure allowed</li></ul></div>	
Functionality Check	<div>Run this query command from the terminal.  *idn?  This should return the Manufacturer, Model number, Serial number, and Firmware version.  GW, GSP-830, P920130, V3.01</div>	

# Command Syntax

The commands are partially compatible with IEEE488.2 (1992) and SCPI (1994) standard. Commands are NON-case sensitive.

Example command

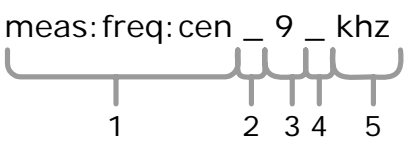

Command Header	1: Command Header	2: Single space
	3: Parameter1	4: Single space
	5: Parameter2	
Command Header	Several command header elements (nodes) can be concatenated to form a complex command. The above example can be separated into: meas: (root node) + freq: + cen:	
Parameter example	0/1	0 or 1.
	1~4	Integer between 1, 2, 3, or 4.
	0.01~5	Decimal number between 0.01 and 5.
	khz	Unit (non-case sensitive)
Message Terminator	Marks the end of a command line. Any of the following is acceptable.	
	CR^END	Line feed code (hexadecimal 0D) with END message
	CR	Line feed code
	<dab>^END	Last data byte with END message
Message Separator	;(semicolon)	Command separator.

## Command Set

- Commands are **non**-case sensitive.
- Underline means a single space (100\_mhz→100 mhz).

### Frequency

meas:freq:cen?	Returns the center frequency in kHz. Example: 1000000 khz
meas:freq:cen	Sets the center frequency. Example: meas:freq:cen_100_mhz
meas:freq:st?	Returns the start frequency in kHz. Example: 1000000 khz
meas:freq:st	Sets the start frequency. Example: meas:freq:st_100_mhz
meas:freq:stp?	Returns the stop frequency in kHz. Example: 1000000 khz
meas:freq:stp	Sets the stop frequency. Example: meas:freq:stp_100_mhz
meas:freq:ss?	Returns the frequency step size in kHz. Example: 1000000 khz
meas:freq:ss	Sets the frequency step. Example: meas:freq:ss_100_mhz
meas:freq:cen:fw	Moves the center frequency one step size forward.
meas:freq:cen:bw	Moves the center frequency one step size backward.

### Span

meas:span?	Returns the frequency span. Example: 10000 khz
meas:span	Sets the frequency span. Example: meas:span:10_mhz
meas:span:full	Sets the frequency span to full.
meas:span:zero	Sets the frequency span to zero.
meas:span:last	Recalls the last frequency span setting.

## Amplitude

meas:refl:unit?	Returns the reference level unit. Parameter: 1 (dBm), 2 (dBmV), 3 (dBuV)
meas:refl:unit	Sets the reference level unit. Parameter: 1 (dBm), 2 (dBmV), 3 (dBuV) Example: meas:refl:unit: 1 (dBm)
meas:refl?	Returns the reference level in current unit. Example: -30 (-30dBm when the unit is dBm)
meas:refl	Sets the reference level in current unit. Example: meas:refl: -30 (-30dBm when in dBm)
meas:refl:scale?	Returns the amplitude scale. Parameter: 1(10dB/Div), 2(5dB/Div), 3(2dB/Div), 4(1dB/Div)
meas:refl:scale	Sets the amplitude scale. Parameter: 1(10dB/Div), 2(5dB/Div), 3(2dB/Div), 4(1dB/Div) Example: meas:refl:scale 1 (10dB/Div)
meas:refl:exg?	Returns the external gain/loss in dB. Example: -6 (-6dB)
meas:refl:exg	Sets the external gain/loss in dB. Example: meas:refl:exg -6 (-6dB)
meas:refl:corr:edit	Sets the amplitude correction data (frequency, amplitude). Need to specify the table index and the number of correction. Example: meas:refl:corr:edit 1_CR 2,100,-40,150,-30 (table index1, 2 data, 100MHz/-40dB, 150MHz/-30dB)
meas:refl:corr:edit:del	Deletes an amplitude correction point. Need to specify set index and point index. Example: meas:refl:corr:edit:del 5_30 (delete set 5, point 30)
meas:refl:corr:edit:delall	Deletes all point in an amplitude correction set. Need to specify set index. Example: meas:refl:corr:edit:delall 5 (delete set No.5)
meas:refl:corr:edit:quit	Quits the amplitude correction mode.
meas:refl:corr:on?	Returns the activated amplitude correction set. Parameter: none, 1 ~ 5 (correction set)
meas:refl:corr:on?	Returns the amplitude correction set is active or inactive. Need to specify the set index. Parameter: on, off Example: meas:refl:corr:on 1? (set No.1 is activated?)
meas:refl:corr:on	Activates the amplitude correction set. Specify the set index. Example: meas:refl:corr:on 1 (activate set No.1)
meas:refl:corr:off	Deactivates the amplitude correction set. Specify set index. Example: meas:refl:corr:off 1 (deactivate set No.1)
meas:inputz?	Returns the input impedance. Parameter: 50, 75

meas:inputz	Sets the input impedance. Parameter: 50, 75 Example: meas:inputz_50 (50Ω)
meas:inputz:cal?	Returns the input impedance calibration value in dB.
meas:inputz:cal	Sets the input impedance calibration value in dB. Example: meas:inputz:cal_5.9 (5.9dB)

## Autoset

meas:autoset:run	Runs autoset.
meas:autoset:amp: auto	Sets the autoset amplitude floor setting to auto mode.
meas:autoset:amp: man	Sets the autoset amplitude floor setting to manual mode. Need to specify the amplitude in dB. Example: meas:autoset:amp:man_20 (20dB)
meas:autoset:amp: mode?	Returns the autoset amplitude floor setting mode. Parameter: auto, manual
meas:autoset:span: auto	Sets the autoset frequency span setting to auto mode.
meas:autoset:span: man	Sets the autoset frequency span setting to manual mode. Need to specify the unit. Example: meas:autoset:span:man_100_khz (100kHz)
meas:autoset:span: mode?	Returns the autoset frequency span setting mode. Parameter: auto, manual

## Marker & Peak Search

meas:mark:on?	Returns marker On/Off. Need to specify the marker ID. Parameter: on, off Example: meas:mark:on_1? (marker 1 On?)
meas:mark:on	Turn On marker. Parameter: 1~5 (marker ID), all (all markers) Example: meas:mark:on_1 (marker 1 On)
meas:mark:off	Turn Off marker. Parameter: 1 ~ 5 (marker ID), all (all markers) Example: meas:mark:off_1 (marker 1 Off)
meas:mark:norm	Sets a marker to normal mode. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:norm_1 (marker 1 normal mode)
meas:mark:norm: freq?	Returns the frequency of a normal marker. Need to specify the marker ID. Example: meas:norm:freq_1? (normal marker 1 frequency?)
meas:mark:norm: level?	Returns the amplitude of a normal marker. Need to specify the marker ID. Example: meas:norm:level_1? (normal marker 1 amplitude?)

meas:mark:delta	Sets a marker to delta mode. Also sets the relative frequency. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:delta_1 (marker 1 in delta mode) Example: meas:mark:delta_1_10_mhz (marker 1 in delta mode, relative frequency 10MHz)
meas:mark:delta:freq?	Returns the relative frequency of a delta marker. Need to specify the marker ID. Example: meas:delta:freq_1? (frequency of delta marker 1?)
meas:mark:delta:level?	Returns the relative amplitude of a delta marker. Need to specify the marker ID. Example: meas:delta:level_1? (amplitude of delta marker 1?)
meas:mark:tomin	Moves a marker to minimum peak. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tomin_1 (marker 1 to minimum peak)
meas:mark:topeak	Moves a normal/delta marker to the peak. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:topeak_1 (marker 1 to peak)
meas:mark:tonp	Moves a normal/delta marker to the next peak. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tonp_1 (marker 1 to the next peak)
meas:mark:tonpr	Moves a normal/delta marker to the next right peak. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tonpr_1 (marker 1 to the next right pk)
meas:mark:tonpl	Moves a normal/delta marker to the next left peak. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tonpl_1 (marker 1 to the next left peak)
meas:mark:tocen	Moves a normal/delta marker to the center frequency. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tocen_1 (marker 1 to the center freq)
meas:mark:tost	Moves a normal/delta marker to the start frequency. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tost_1 (marker 1 to the start frequency)
meas:mark:tostp	Moves a normal/delta marker to the stop frequency. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:tostp_1 (marker 1 to stop frequency)
meas:mark:toss	Moves a normal/delta marker to the center frequency + step. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:toss_1 (marker 1 to center freq + step)
meas:mark:torefl	Moves a normal/delta marker to the reference level. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:torefl_1 (marker 1 to the reference level)
meas:mark:trace	Moves a normal/delta marker to a trace. Parameter: 1 ~ 5 (marker ID), followed by 0 (auto), 1 (traceA), 2 (traceB), 3 (traceC) Example: meas:mark:trace_1_2 (marker 1 to traceB)



meas:mark: marktable:on	Activates marker table.
meas:mark: marktable:off	Deactivates marker table.
meas:mark: peaktable:on	Activates peak table.
meas:mark: peaktable:off	Deactivates peak table.
meas:mark: peaktable:sortf	Sorts peak table by frequency.
meas:mark: peaktable:sorta	Sorts peak table by amplitude.
meas:mark: peaktrack:on	Turns On peak track. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:peaktrack:on_1 (marker 1 tracks peak)
meas:mark: peaktrack:off	Turns Off peak track. Parameter: 1 ~ 5 (marker ID) Example: meas:mark:peaktrack:off_1 (marker 1 no more tracks peak)
meas:mark: peakthres:on	Turns On peak threshold and sets amplitude. Parameter: peak threshold in dB. Example: meas:mark:peakthres:on_-30 (-30dB threshold)
meas:mark: peakthres:off	Turns Off peak threshold.

## Trace

meas:tra	Sets the mode for a trace. Parameter: 1 (traceA), 2 (traceB), 3 (traceC), followed by 1 (clear), 2 (peak hold), 3 (view), 4 (blank) Example: meas:tra_1_2 (traceA set to peak hold mode)
meas:tra:avg:on	Turns On average mode and sets average number for a trace. Parameter: 1(traceA), 2(traceB), 3(traceC), followed by No. Example: meas:tra:avg:on_1_20 (Average trace A 20 times)
meas:tra:avg:off	Turns Off the average mode. Parameter: 1 (traceA), 2 (traceB), 3 (traceC) Example: meas:tra:avg:off_1 (traceA average mode Off)
meas:tra:read?	Returns trace data. Parameter: 1(traceA), 2(traceB), 3(traceC), all(all three traces) Example: meas:read_1? (traceA data)
meas:tra:a<>b	Swaps trace A and B.
meas:tra:a+b>a	Adds trace B to A.
meas:tra:a-b>a	Subtracts trace B from A.

meas:tra:const?	Returns the constant value to be added or subtracted.
meas:tra:const	Sets the constant value to be added or subtracted.
meas:tra:a+const>a	Adds a constant value to traceA.
meas:tra:a—const>a	Subtracts a constant value from traceA.
meas:tra:det?	Returns the detection mode. Parameter: 1(normal), 2(sample), 3(peak+), 4(avg), 5(qpeak)
meas:tra:det	Sets the detection mode. Parameter: 1(normal), 2(sample), 3(peak+), 4(avg), 5(qpeak) Example: meas:tra:det_4 (set the detection mode to average)

## Power measurement

meas:ch:bw?	Returns the main channel bandwidth. Example: 1000 khz
meas:ch:bw	Sets the main channel bandwidth. Need to specify the unit. Example: meas:ch:bw_1_mhz (1MHz)
meas:adjc:bw?	Returns the adjacent channel bandwidth in kHz. Need to specify the channel. Example: meas:adjc:bw_2? (adjacent channel2 bandwidth)
meas:adjc:bw	Sets the adjacent channel bandwidth. Need to specify the channel and unit. Example: meas:adjc:bw_2_1_mhz (adjacent channel2 bandwidth 1MHz)
meas:adjc:offs?	Returns the adjacent channel offset in kHz. Specify channel. Example: meas:adjc:offs_2? (adjacent channel2 offset)
meas:adjc:offs	Sets the adjacent channel offset. Specify channel and unit. Example: meas:adjc:offs_2_1_mhz (adjacent ch2 offs 1MHz)
meas:acpr?	Returns ACPR measurement activation status. Parameter: on, off
meas:acpr	Turns On/Off ACPR measurement. Parameter: on, off Example: meas:acpr_on (ACPR On)
meas:acpr:lower?	Returns the lower ACPR result. Need to specify 1 or 2. Example: meas:acpr:lower_2? (lower ACPR 2 result?)
meas:acpr:upper?	Returns the upper ACPR result. Need to specify 1 or 2. Example: meas:acpr:upper_2? (upper ACPR 2 result?)
meas:acpr:chup	Moves the ACPR channel up.
meas:acpr:chdown	Moves the ACPR channel down.
meas:chspc?	Returns the channel space in kHz.
meas:chspc	Sets the channel space. Need to specify the unit. Example: meas:chspc_10_mhz (10MHz)
meas:ocbw?	Returns the OCBW activation/deactivation status. Parameter: on, off

meas:ocbw	Turns On/Off OCBW. Parameter: on, off Example: meas:ocbw_on
meas:ocbw:bw?	Returns the power measurement channel space in kHz.
meas:ocbw:per?	Returns OCBW percentage.
meas:ocbw:per	Sets OCBW percentage. Example: meas:ocbw:per_90 (90%)
meas:ndb?	Returns N dB activation/deactivation status. Parameter: on, off
meas:ndb	Turns On/Off N dB. Parameter: on, off Example: meas:ndb_on
meas:ndb:ndb?	Returns N dB.
meas:ndb:ndb	Sets N dB. Example: meas:ndb:ndb_3 (3 dB)
meas:ndb:bw?	Returns N dB bandwidth. Example: 1000 khz
meas:jitter?	Returns Phase Jitter activation/deactivation status. Parameter: on, off
meas:jitter	Turns On/Off Phase Jitter. Parameter: on, off Example: meas:jitter_on
meas:jitter:stoffs?	Returns Phase Jitter start offset. Example: 0 khz
meas:jitter:stoffs	Sets Phase Jitter start offset. Need to specify the unit. Example: meas:jitter:stoffs_0_khz
meas:jitter:stpoffs?	Returns Phase Jitter stop offset. Example: 50 khz
meas:jitter:stpoffs	Sets Phase Jitter stop offset. Need to specify the unit. Example: meas:jitter:stpoffs_50_khz
meas:jitter:phase?	Returns Phase Jitter phase result in radian. Example: 1.234 rad
meas:jitter:time?	Returns Phase Jitter time result in pico second. Example: 1.234 psec

## Limit line

meas:lmeline:on	Turns On limit line. Parameter: 0 (low limit line), 1 (high limit line) Example: meas:lmeline:on_0 (low limit line On)
meas:lmeline:off	Turns Off limit line. Parameter: 0 (low limit line), 1 (high limit line) Example: meas:lmeline:off_0 (low limit line Off)

meas:limitline:passfail	Turns On/Off Pass/Fail test. Parameter: on, off Example: meas:limitline:passfail_on (Pass/Fail test On)
meas:limitline: passfail:criterion?	Returns Pass/Fail test criteria. Parameter: 1 (pass if all signals are in the zone), 2 (pass if the peaks are in the zone), 3 (pass if valleys are in the zone)
meas:limitline: passfail:criterion	Sets Pass/Fail test criteria. Parameter: 1 (pass if all signals are in the zone), 2 (pass if the peaks are in the zone), 3 (pass if valleys are in the zone) Example: meas:limitline:passfail:criterion_3
meas:limitline:table?	Returns limit line table On/Off. Parameter: on, off
meas:limitline:table	Turns On/Off limit line table. Parameter: on, off Example: meas:limitline:table_on (limit line table On)
meas:limitline:edit	Sets the limit line table data. Need to specify 0 (low limit line), 1 (high limit line) / limit line points. Example: meas:limitline:edit_0_CR_3,100,-20,110,-30,120,-25 (low limit line, 3 points, 100MHz/-20dB, 110MHz/-30dB, 120MHz/-25dB)
meas:limitline:edit: delall	Delete all points in limit line table. Parameter: 0 (low limit line), 1 (high limit line) Example: meas:limitline:edit:delall_0 (delete low limit line table)

## BW

con:rbw:auto	Sets RBW to auto.
con:rbw?	Returns the RBW (resolution bandwidth). Parameter: 0 (10kHz), 1 (300Hz), 2 (3kHz), 3 (9kHz), 4 (30kHz), 5 (120kHz), 6 (300kHz), 7 (4MHz), 8 (100kHz)
con:rbw:man	Selects the RBW. Parameter: 0 (200Hz), 1 (300Hz), 2 (3kHz), 3 (9kHz), 4 (30kHz), 5 (120kHz), 6 (300kHz), 7 (4MHz) Example: con:rbw:man_1 (sets RBW to 300Hz)
con:rbw:mode?	Returns RBW mode. Parameter: auto, manual
con:vbw:auto	Sets VBW to auto.
con:vbw?	Returns the VBW (video bandwidth). Parameter: 0 (10Hz), 1 (30Hz), 2 (100Hz), 3 (300Hz), 4 (1kHz), 5 (3kHz), 6 (10kHz), 7 (30kHz), 8 (100kHz), 9 (300kHz), 10 (1MHz)
con:vbw:man	Selects the VBW. Parameter: 0 (10Hz), 1 (30Hz), 2 (100Hz), 3 (300Hz), 4 (1kHz), 5 (3kHz), 6 (10kHz), 7 (30kHz), 8 (100kHz), 9 (300kHz), 10 (1MHz) Example: con:vbw:man_4 (sets VBW to 1kHz)
con:vbw:mode?	Returns VBW mode. Parameter: auto, manual
con:swt:auto	Sets the sweep time to auto.
con:swt:man	Sets the sweep time in msec. Example: con:swp:man_5 (sets the sweep time to 5ms)
con:swt:mode?	Returns the sweep time mode. Parameter: auto, manual
con:allcouple	Sets the RBW, VBW, and sweep time to auto.

## Trigger

con:trig:freerun	Sets the trigger to free run mode.
con:trig:video	Sets the trigger to video mode. Also sets the trigger level in current unit. Example: con:trig:video_-20 (video mode On, -20dBm)
con:trig:single	Sets the trigger condition to single.
con:trig:cont	Sets the trigger condition to continuous.
con:trig:ext	Sets the trigger to external mode.
con:trig:delay	Sets the trigger delay in msec. Example: con:trig:delay_1000 (1000ms delay)
con:trig:freq	Sets the trigger frequency in MHz. Example: con:trig:freq_1 (1MHz)

## Display

con:disp:dim	Selects the display dimmer level. Parameter: 0 ~ 5 Example: con:disp:dim_2 (dimmer level 2)
con:disp:dl	Turns On/Off display line. Parameter: on, off Example: con:disp:dim_on (display line On)
con:disp:dl:level	Sets the display line level in current unit. Example: con:disp:dl:level_-50 (display line at -50dBm)
con:disp:title:show	Sets and shows the display title. The title is case sensitive. Example: con:disp:title:show_SAtest (title is SAtest)
con:disp:title:clr	Clears the display title.
con:disp:split:upper	Turns On and sweeps upper window in split window mode.
con:disp:split:lower	Turns On and sweeps lower window in split window mode.
con:disp:split:alt	Sweeps the upper and lower window alternatively in split window mode.
con:disp:split:full	Goes back to full screen mode.

## File

con:file:copy:typesel	Selects the type of copied file. Parameter: 0 (trace), 1 (limit line), 2 (correction), 3 (sequence), 4 (setup) Example: con:file:copy:typesel_2 (copy amplitude correct file)
con:file:copy	Copies file. Need to specify the source and destination file. Parameter: ta/tb/tc (traceA/B/C), tl~l0 (tracel~l0), lh/lI (high/low limit line), lhI~5 (high limit line 1~5), llI~5 (low limit line 1~5), cl~5 (correction set 1~5), ql~l0 (sequence 1~l0), file name in external USB flash drive Example: con:file:copy_tl0_ta (copy from tracel0 to traceA) Example: con:file:copy_ta_mytrace (copy from traceA to a file in external USB flash named mytrace)
con:file:del:typesel	Deletes the type of copied file. Parameter: 0 (trace), 1 (limit line), 2 (correction), 3 (sequence), 4 (setup) Example: con:file:del:typesel_2 (delete amplitude correct file)
con:file:del	Deletes file. Need to specify the source and destination file. Parameter: ta/tb/tc (traceA/B/C), tl~l0 (tracel~l0), lh/lI (high/low limit line), lhI~5 (high limit line 1~5), llI~5 (low limit line 1~5), cl~5 (correction set 1~5), ql~l0 (sequence 1~l0), file name in external USB flash drive Example: con:file:del_tl0 (delete tracel0) Example: con:file:del_myspace (delete a file names myspace in extrenal USB flash drive)
con:file:rename	Renames a file in external USB flash drive. Need to specify the original and changed name. Example: con:file:rename_myspace_myfile (change a file named myspace to myfile)

con:file:prtsc:tofile	Saves the display image to external USB flash drive. Need to specify the file name. Example: con:file:prtsc:tofile_myscreen (saves the display image to a file named myscreen)
-----------------------	---

## Preset

con:preset	Presets GSP-830.
------------	------------------

## System

con:sys:setup:save	Save the current system setting to setup file. Parameter: 1~10 Example: con:sys:setup:save_1 (save current setup to setup1)
con:sys:setup:recall	Recalls a system setting from setup file. Parameter: 1~10 Example: con:sys:setup:recall_1 (recall setting in setup1 file)
con:sys:gpibaddr?	Returns the current GPIB address.
con:sys:gpibaddr	Sets the GPIB address. Example: con:sys:gpib:addr_2 (set GPIB address to 2)
con:sys:auxsig	Turns On/Off the auxiliary signal. Parameter: on, off Example: con:sys:auxsig_on (auxiliary signal On)
con:sys:clock:date?	Returns the current date setting. Parameter: year / month / day / day of week 1 (Sun) ~ 7 (Sat) Example: 2006 6 24 7 (June 24 <sup>th</sup> , Saturday, 2006)
con:sys:clock:date	Sets the date. Parameter: year / month / day / day of week 1 (Sun) ~ 7 (Sat) Example: con:sys:clock:date_2006_6_24_7 (Jun24, Sat, 2006)
con:sys:clock:time?	Returns the current time setting. Parameter: hour / minute / second Example: 13 30 26 (1p.m., 30 minutes, 26 second)
con:sys:clock:time	Sets the time. Parameter: hour / minute / second Example: con:sys:clock:time_13_30_26 (1p.m., 30min, 26sec)
con:sys:clock:show	Turns On/Off clock display. Parameter: on, off Example: con:sys:clock:show_on (clock display On)
con:sys:selftest?	Returns the self test result. Parameter: 0 (fail), 1 (pass) in the following order: GPIB/Flash/SDRAM/RTC Example: 1 1 0 1 (GPIBpass,Flashpass,SDRAMfail,RTCpass)
con:sys:lang	Selects language. Parameter: 1 (English), 2 (Simplified Chinese) Example: con:sys:lang_2 (switch to simplified Chinese)
con:sys:ser?	Returns the serial number. Example: EE8300000

con:sys:swver?	Returns the software version. Example: 01.00 06/07/28 (version 1.00, 2006 July 28 <sup>th</sup> )
con:sys:fwver?	Returns the firmware version. Example: 01.00 (version 1.00)
con:sys:hwver?	Returns hardware version in following order. RF, IF, DSP, MB Example: 01.00 01.00 01.01 01.00 (RF: version 1.00, IF: version 1.00, DSP: version 1.01, MB: version 1.00)
con:sys:optstatus?	Returns optional items installation status in the following order. 300HzRBW, EMIFilter, 10k/100kHzRBW, TG, Demodulator, Medref ( $\pm 1$ ppm stability) Parameter: 0 (not installed), 1 (installed) Example: 0 0 1 1 1 (TG, Demodulator, Medref are installed)

## Option

con:opt:tg	Turns On/Off Tracking Generator (TG). Parameter: on, off Example: con:opt:tg_on (TG On)
con:opt:tg:level?	Returns the TG level.
con:opt:tg:level	Sets the TG level.
con:opt:tg:norm	Turns On/Off TG normalization. Parameter: on, off Example: con:opt:tg:norm_on (normalization On)
con:opt:tg:offset	Sets the TG offset level.
con:opt:ge:refval?	Returns the TG reference value.
con:opt:ge:refval	Sets the TG reference value.
con:opt:dm:fm	Turns On/Off FM in the demodulator. Parameter: on, off Example: con:opt:dm:fm_on (FM On)
con:opt:dm:am	Turns On/Off AM in the demodulator. Parameter: on, off Example: con:opt:dm:am_on (AM On)
con:opt:dm:spk	Turns On/Off phone output in the demodulator. Parameter: on, off Example: con:opt:dm:spk_on (phone output On)
con:opt:dm:vol	Sets the demodulator phone output volume.
con:opt:dm:sql?	Returns the demodulator squelch level.
con:opt:dm:sql	Sets the demodulator squelch level.
con:opt:bat?	Returns the battery level.
con:opt:extreffreq?	Returns the external reference frequency.
con:opt:extreffreq	Sets the external reference frequency.

## Sequence



con:seq:runmode	Selects the sequence run mode. Parameter: 1 (repeat mode), 2 (single mode) Example: con:seq:runmode_2 (sequence runs in sing mode)
con:seq:runseq	Runs the sequence. Parameter: sequence index, 1 ~ 10 Example: con:seq:runseq_2 (run sequence 2)
con:seq:stopseq	Stops the running sequence.
con:seq:delallseq	Deletes all programmed sequence.
con:seq:delseq	Deletes a sequence. Parameter: sequence index, 1 ~ 10 Example: con:seq:delseq_2 (delete sequence 2)

# F

## FAQ

- I pressed the Power (On/Standby) key on the front panel but nothing happens.
- I cannot even see the default green line on the display.
- I connected the signal but it does not appear on screen.
- I want to see which optional items are installed.
- The GSP-830 performance does not match the specification.

---

I pressed the Power (On/Standby) key on the front panel but nothing happens.

Make sure you turned On the rear panel Power switch.  
For details, see page22.

Note that after proper sequence, it takes around 10  
seconds for the display to become active.

---

I cannot even see the default green line on the display.

Check if the Trace Blank (hide trace from the display) is  
On for TraceA, the default waveform. Press the Trace  
key→F1 (select TraceA)→F2 (Clear) to recover the trace.  
For details, see page76.

---

I connected the signal but it does not appear on screen.

Run the Autoset and let GSP-830 find the best display  
scale for your target signal. Press the Autoset key, then  
press F1 (Autoset). For details, see page60.

---

I want to see which optional items are installed.

Check the optional item status in the system information  
window. Press the System key → F6 (More) → F4  
(System Config On). For details, see page132.

The Pre-amplifier (page58) is a completely external item,  
therefore does not appear in the system information  
menu.

---

The GSP-830 performance does not match the specification.

Make sure the device is powered On for at least 30 minutes, within +20°C~+30°C. This is necessary to stabilize the unit to match the specification.

---

If there is still a problem, please contact your local dealer or GWInstek at [marketing@goodwill.com.tw](mailto:marketing@goodwill.com.tw).

# Appendix

## GSP-830 Specification

Frequency	Frequency Range	9kHz ~ 3.0GHz
	Aging Rate	$\pm 10$ ppm, 0-50° C, 5ppm/yr
	Span Range	2kHz ~ 3.0GHz in 1/2/5 sequence, full span, zero span
	Phase Noise	-80dBc/Hz @ 1GHz 20kHz Offset typ.
	Sweep Time Range	50 ms ~ 25.6s
Resolution Bandwidth	RBW Range	3kHz, 30kHz, 300kHz, 4MHz
	RBW Accuracy	15%
	VBW Range	10Hz ~ 1MHz in 1-3 steps
Amplitude	Measurement Range	-103dBm ~ +20dBm: 1 MHz ~ 15MHz, Ref Lvl @ -30dBm -120 $\pm$ 1dBm ~ +20dBm: 15MHz ~ 600MHz, Ref Lvl @ -50dBm -117 $\pm$ 1dBm ~ +20dBm: 600MHz ~ 2.3GHz, Ref Lvl @ -50dBm -115 $\pm$ 1dBm ~ +20dBm: 2.3GHz ~ 3GHz, Ref Lvl @ -50dBm
		Overload Protection +30dBm, 25VDC
		Reference Level Range -110dBm ~ +20dBm
		Accuracy $\pm 1$ dB @ 100MHz
		Frequency Flatness $\pm 1$ dB
		Display Range Linearity $\pm 1$ dB over 70dB
	Average Noise Floor	-135dBm/Hz: 1MHz ~ 15MHz, Ref Lvl @ -30dBm -152 $\pm$ 1dBm/Hz: 15MHz ~ 600MHz, Ref Lvl @ -50dBm -149 $\pm$ 1dBm/Hz: 600MHz ~ 2.3GHz, Ref Lvl @ -50dBm -147 $\pm$ 1dBm/Hz: 2.3GHz ~ 3GHz, Ref Lvl @ -50dBm
		Third Intermodulation <-70dBc @ -40dBm Input, Ref Level $\geq$ -30dBm
	Harmonic Distortion <-60dBc RF Input < -40dBm,	

General	Non-Harmonic Spurious	Ref Level @ -30dBm ≤ -93dBm: 1MHz~15MHz, RefLvl @ -30dBm ≤ -109dBm: 15MHz~600MHz, RefLvl @ -50dBm ≤ -106dBm: 600MHz~2.3GHz, RefLvl @ -50dBm ≤ -104dBm: 2.3GHz~3GHz, RefLvl @ -50dBm
	Display	640 x 480 high-res color TFT LCD
	Internal Memory	10 Traces, 10 Setup Info, 10 Limit Lines, 5 Corrections, 10 Sequences
	Markers	10 markers for peaks: 5 normal-delta marker pairs Functions: Delta, Peak, Marker Track
	Trace Detection	3 traces with Peak, Maximum hold, Freeze, Average, and Trace Math
	Power Measurement	ACPR, OCBW, Channel power, N dB BW, and Phase Jitter
	Autoset Function	Auto tuning the measurement result for observation
	Sequence	Automated test by user defined macros without any remote control
Connectors	RF Input	Type: N Female, 50Ω nominal RF input VSWR: <2:1, @Ref Lvl 0dBm
	External Reference Clock Input	Type: BNC Female, 1M, 1.544M, 2.048M, 5M, 10M, 10.24M, 13M, 15.36M, 15.4M, 19.2M
	External Trigger Input	Type: BNC Female, +5V TTL signal
	Ref. Clock Output	Type: BNC Female, 10MHz
	DC Input	Jack: 5.5mm, 12V
	RS-232C	D-Sub 9pins Female
	VGA Output	D-Sub 15pins Female
	USB Connector	Front Panel: Type A Rear Panel: Type B mini
	DC Voltage Output	SMB Male, +9V/100mA max output
Power Source	AC Input	100V ~ 240V, 50/60Hz
Accessories	Contents	User Manual x1, Power Cord x1
Dimensions & Weight	Dimension	330 (W) × 170(H) × 340(D) mm
	Weight	Approx. 6kg / Full Option Installed
Atmospherics	Ambient Temperature	18°C ~ 28°C for operation 0°C ~ 40°C for storage
	Relative Humidity	<90% for operation

註解 [IK2]:

&lt;85% for storage

## Optional Items Specifications

Opt.01 Tracking Generator (*2)	Frequency Range	9kHz ~ 3.0GHz
	Amplitude Range	-50dBm ~ 0 dBm
	Amplitude Accuracy	$\pm 1$ dB @100MHz, 0dBm
	Amplitude Flatness	$\pm 1$ dB @0dBm
	Harmonics	<-30dBc typical
	Reverse Power	+30dBm
	Impedance	Type: N female, 50 $\Omega$ nominal
	TG Output VSWR	< 2:1
Opt.02 Battery Pack	Battery Type	11.1V Li-Ion battery pack x 2
Opt. 03 $\pm 1$ ppm Stability (*2)	Output Range	$\pm 1$ ppm, 0~50°C
	Aging Rate	$\pm 1$ ppm / year
Opt. 04 300Hz RBW (*2)	RBW Selection	300Hz, 3dB bandwidth
	RBW Accuracy	20%
Opt. 05 9kHz & 120kHz RBW (*1, 2)	RBW Selections	9kHz and 120kHz, 6dB bandwidth
	RBW Accuracy	15%
Opt. 06 10kHz & 100kHz RBW (*1, 2)	RBW Selections	10kHz and 100kHz, 3dB bandwidth
	RBW Accuracy	15%
Opt. 07 AM/FM Demodulator and 10kHz & 100kHz RBW (*1, 2)	Demodulation	AM, FM
	Output	Internal Speaker, 3.5mm stereo jack wired for mono operation
	RBW Selections	10kHz and 100kHz, 3dB bandwidth
	RBW Accuracy	15%
Opt. 08 GPIB Interface	Compliant standard	IEEE 488.2 bus
GKT-001 General Kit Set	ADP-002	SMA (J/F) to N (P/M) adaptor x 2
	ATN-100	10dB Attenuator, N (J)~N(P) x 1
	GTL-303	RF Cable assembly (RD316, SMA(P), 60cm) x 2
	GSC-002	Kit box x 1
GKT-002 CATV Kit set	ADP-001	BNC (J/F) to N (P/M) adaptor x 2

	ADP-101	BNC (P/M) 50Ω to BNC (J/F) 75Ω adaptor x 2
	GTL-304	RF Cable assembly (RG223, N(P)-N(J), 30cm) x 2
	GSC-003	Kit box x 1
GKT-003 RLB Kit set	GAK-001	Termination, 50Ω, N(P) x 1
	GAK-002	Cap with chain, N(P) x 1
	GTL-302	RF Cable assembly (RG223+N(P), 30cm) x 2
	GSC-004	Kit box x 1
GTL-401 DC Power Cord	DC power cord with DC Jack and lighter plug, current 5A	
GAP-801 10dB Preamplifier	Frequency range	9kHz ~ 6GHz
	Gain	10dB typical
GSC-001 Soft Carrying Case	Soft Carrying Case	

\* Note:

1. Among Opt. 05 to 07, only one item can be installed to given GSP-830.
2. The following are factory installed items. Opt. 01, 03, 04, 05, 06, 07

## Declaration of Conformity

We

**GOOD WILL INSTRUMENT CO., LTD.**

(1) No.7-1, Jhongsing Rd., Tucheng City, Taipei County, Taiwan

(2) No. 69, Lu San Road, Suzhou City (Xin Qu), Jiangsu Sheng, China

declare, that the below mentioned product

**Type of Product: Digital Spectrum Analyzer**

**Model Number: GSP-830**

are herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (89/336/EEC, 92/31/EEC, 93/68/EEC) and Low Voltage Directive (73/23/EEC, 93/68/EEC).

For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Directive, the following standards were applied:

### ◎ EMC

EN 61326-1: Electrical equipment for measurement, control and laboratory use — EMC requirements (1997 + A1:1998 + A2:2001 + A3:2003)

Conducted Emission	Electrostatic Discharge
Radiated Emission	EN 61000-4-2: 1995 + A1:1998 + A2:2001
EN 55011: Class A 1998 + A1:1999 + A2:2002	

Current Harmonics	Radiated Immunity
EN 61000-3-2: 2000 + A2:2005	EN 61000-4-3: 2002 + A1:2002

Voltage Fluctuations	Electrical Fast Transients
EN 61000-3-3: 1995 + A1:2001	EN 61000-4-4: 2004

-----	Surge Immunity
	EN 61000-4-5: 1995 + A1:2001

-----	Conducted Susceptibility
	EN 61000-4-6: 1996 + A1:2001

-----	Power Frequency Magnetic Field
	EN 61000-4-8: 1993 + A1:2001

-----	Voltage Dip/ Interruption
	EN 61000-4-11: 2004

### ◎ Safety

Low Voltage Equipment Directive 73/23/EEC

Safety Requirements

IEC/EN 61010-1: 2001



# INDEX

## A

ACPR .....	85
activate, marker .....	64
amplitude	
chapter .....	49
command set .....	166
menu tree .....	33, 34
operation shortcut .....	27
peak sort .....	74
specification .....	180
amplitude correction .....	53
file type .....	117
amplitude floor, Autoset .....	62
Autoset	
chapter .....	60
command set .....	167
in functionality check .....	24
menu tree .....	33
operation shortcut .....	27
auxiliary signal .....	24
average	
detection .....	83
trace .....	77
waveform .....	104

## B

bandwidth	
chapter .....	98
command set .....	173
menu tree .....	37
operation shortcut .....	30
specification .....	180

## battery

chapter .....	151
safety instruction .....	8
specification .....	182

## C

### CATV

impedance selection .....	59
kit set .....	183
center and span .....	43
center frequency .....	43
move marker to .....	68
move peak to .....	72
cleaning GSP-830 .....	9
clear trace .....	76
command set, general .....	178
continuous trigger mode .....	108
control keys overview .....	15
copy file .....	118
correction, amplitude .....	53

## D

date setting .....	135
DC operation .....	152
delay, trigger .....	109
delete file .....	121
delta marker .....	66
demodulator	
chapter .....	147
specification .....	182
detection mode .....	82
display	
chapter .....	110

clock activation .....	135
command set .....	174
FAQ .....	178
menu tree .....	37
output .....	114
display icon	
75ohm impedance .....	59
amplitude correction.....	53, 56
battery level .....	152
external offset .....	52
external reference .....	137
internal reference median.....	136
overview.....	21
peak track.....	67, 71
RBW manual.....	99
sequence running.....	144
TG normalized .....	146
trace average.....	78, 105
trace clear mode.....	76
trace math .....	80
trace peak hold.....	77
trace view .....	77
trigger external.....	108
trigger video .....	107
VBW manual.....	101
display line .....	111

## E

EMI filter	
chapter.....	149
RBW selection .....	99
specification.....	182
EN 55011	
declaration of conformity.....	184
EN 61010	
declaration of conformity.....	184
measurement category .....	8
pollution degree .....	9
external offset.....	52

external reference signal.....	137
external trigger .....	108

## F

FAQ.....	178
feature list.....	12
file	
chapter .....	116
command set.....	174
menu tree.....	38
operation shortcut .....	30
rename .....	123
rename copy file.....	120
Flash test result.....	134
free run.....	107
freeze trace.....	77
frequency	
chapter .....	42
command set.....	165
menu tree.....	33
operation shortcut .....	27
peak sort .....	74
specification .....	180
frequency adjustment point .....	17
full span.....	47
functionality check	
instrument .....	24
PC software.....	157
fuse instruction .....	9

## G

GAP-801 .....	58
general kit set .....	182
getting started chapter.....	11
GPIB configuration.....	130, 162

## H

hide trace.....	77
high limit line .....	93
horizontal view range, Autoset .....	62

<b><i>I</i></b>	<b><i>O</i></b>
impedance offset ..... 59	OCBW ..... 88
impedance selection ..... 59	operation environment ..... 9
<b><i>L</i></b>	option
language selection ..... 138	command set ..... 176
last span setting ..... 48	menu tree ..... 40
LCD dimmer ..... 111	operation shortcut ..... 31
limit line	optional item
chapter ..... 92	10/100kHz RBW ..... 99
command set ..... 172	300Hz RBW ..... 99
file type ..... 117	battery ..... 151
menu tree ..... 36	demodulator ..... 147
operation shortcut ..... 29	EMI filter ..... 149
low limit line ..... 93	FAQ ..... 178
<b><i>M</i></b>	installation status ..... 133
main keys overview ..... 14	package content ..... 13
marker	pre-amplifier ..... 58
chapter ..... 63	specification ..... 182
command set ..... 167	TG ..... 145
menu tree ..... 34	overview
operation shortcut ..... 28	characteristics ..... 12
PC software ..... 159	display ..... 20
peak track ..... 71	display icon ..... 21
to trace ..... 78	front panel ..... 14
marker table ..... 69	preset ..... 41, 126
marker to center ..... 68	RBW/VBW setting ..... 102
marker to peak ..... 67	rear panel ..... 17
measurement keys overview ..... 15	<b><i>P</i></b>
minimum peak ..... 73	package content ..... 13
<b><i>N</i></b>	panel setting
N dB ..... 90	file type ..... 118
next peak ..... 72	save/recall ..... 128
normal detection mode ..... 82	pass/fail test ..... 96
normal trigger mode ..... 108	PC requirement ..... 154
numerical keys example ..... 16	PC software chapter ..... 153
	peak hold trace ..... 76
	peak search
	chapter ..... 70

command set .....	167	RLB kit set .....	183
menu tree .....	35	RS-232C configuration .....	129, 155, 162
operation shortcut.....	28	RTC test result .....	134
peak table .....	73		
phase jitter.....	91	<b>S</b>	
phone output.....	147	safety instruction	
positive peak detection .....	82	general guideline .....	8
power measurement		symbol .....	7
chapter.....	84	UK power cord .....	10
command set .....	170	sample detection mode .....	82
menu tree .....	36	SDRAM test result .....	134
operation shortcut.....	29	sequence	
power supply safety instruction .....	8	chapter .....	139
power up sequence .....	22	command set.....	177
FAQ .....	178	file type .....	117
pre-amplifier.....	58	menu tree.....	40
specification.....	183	operation shortcut .....	32
preset		serial number.....	132
chapter.....	126	service operation	
command set .....	175	contact.....	179
operation shortcut.....	31	menu .....	138
printout		signal detection	
display image .....	159	average.....	149
		quasi-peak.....	149
<b>Q</b>		single trigger mode.....	108
quasi-peak detection .....	83	span .....	44
		chapter .....	42
<b>R</b>		command set.....	165
RBW .....	99	menu tree.....	33
reference level .....	50	operation shortcut .....	27
move marker to.....	68	specification .....	180
reference signal		specification	
status .....	133	FAQ .....	179
synchronize with other device.....	136	GSP-830 .....	180
remote access		optional item.....	182
PC software .....	153	split display.....	113
via command set .....	161	squelch, demodulator setting.....	148
remote control chapter.....	161	start and stop.....	45
rename file.....	123	move marker to.....	68

start frequency .....	45	command set.....	169
state keys overview.....	15	FAQ .....	178
step, frequency .....	43, 45	file type .....	117
stop frequency .....	46	menu tree.....	35
storage environment.....	9	move marker to .....	69, 78
sweep time.....	104	operation shortcut.....	28
synchronization		trace math.....	80
master .....	136	trigger	
reference signal status .....	133	chapter.....	106
slave.....	137	command set.....	173
system		menu tree.....	37
chapter .....	127	operation shortcut.....	30
command set .....	175		
configuration window.....	132	<b>U</b>	
error message.....	23, 131	USB	
menu tree .....	39	file copy .....	118
self-test.....	23, 134	file delete .....	121
		file rename.....	123
<b>T</b>		save display image .....	114, 124
table of contents .....	3	slave configuration.....	129, 155, 162
TG			
chapter .....	145	<b>V</b>	
specification .....	182	VBW .....	101
threshold, peak.....	74	version information.....	132
tilt stand.....	22	vertical unit .....	51
time domain view.....	47	VGA output .....	114
time setting .....	135	video trigger.....	107
title, display.....	112		
trace		<b>Z</b>	
chapter .....	75	zero span .....	47